





*Capture 20*

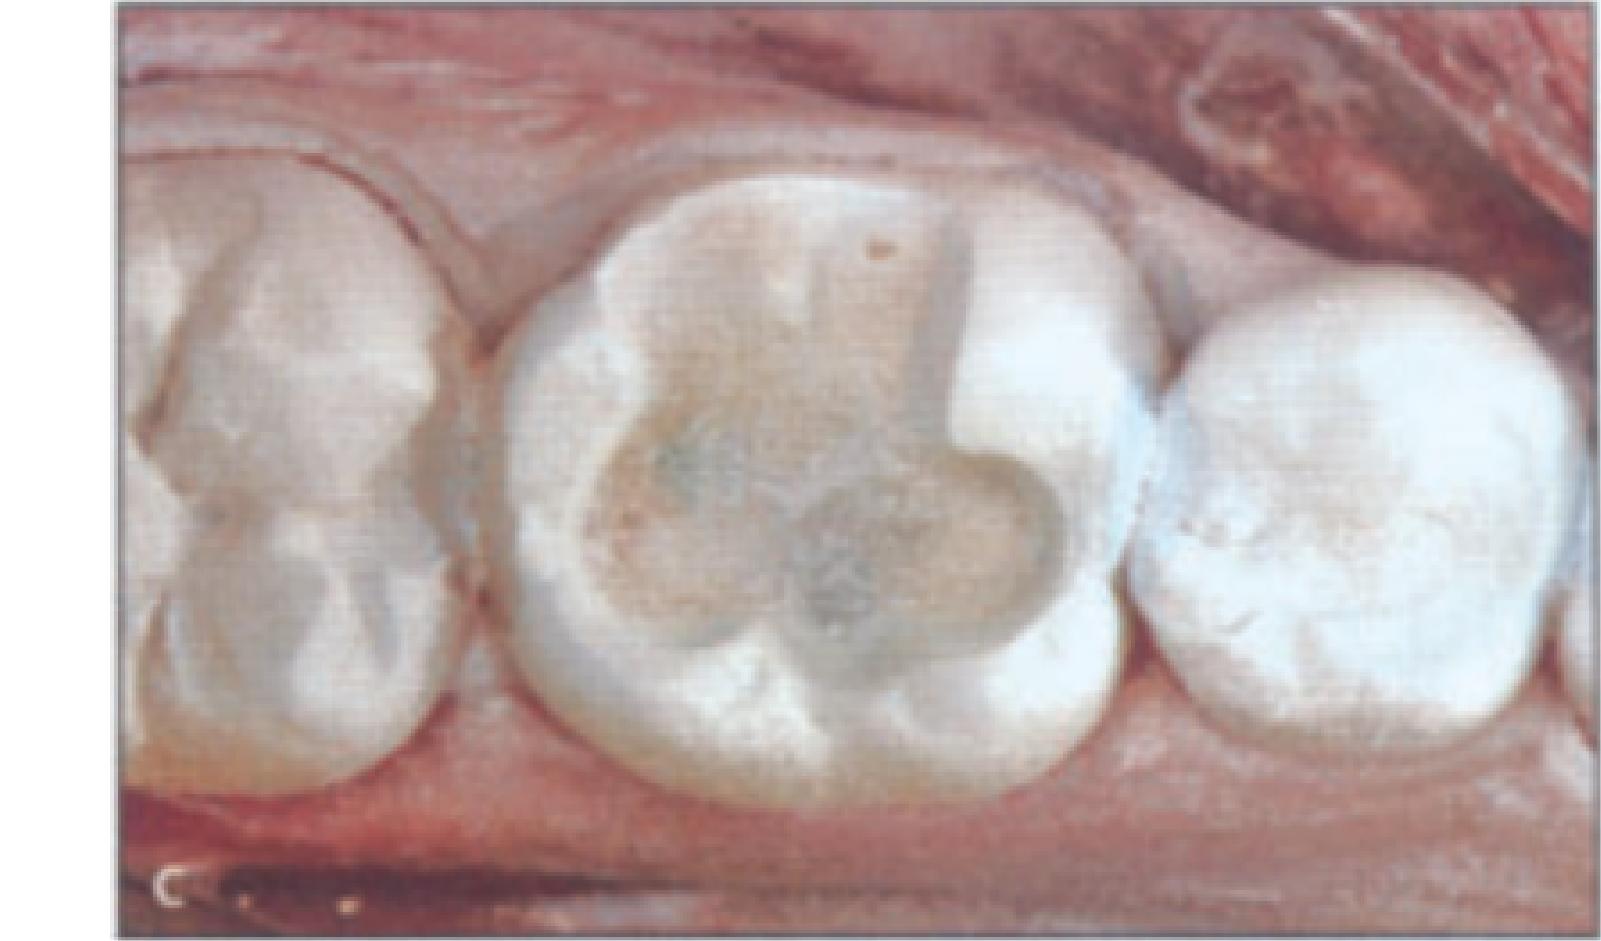

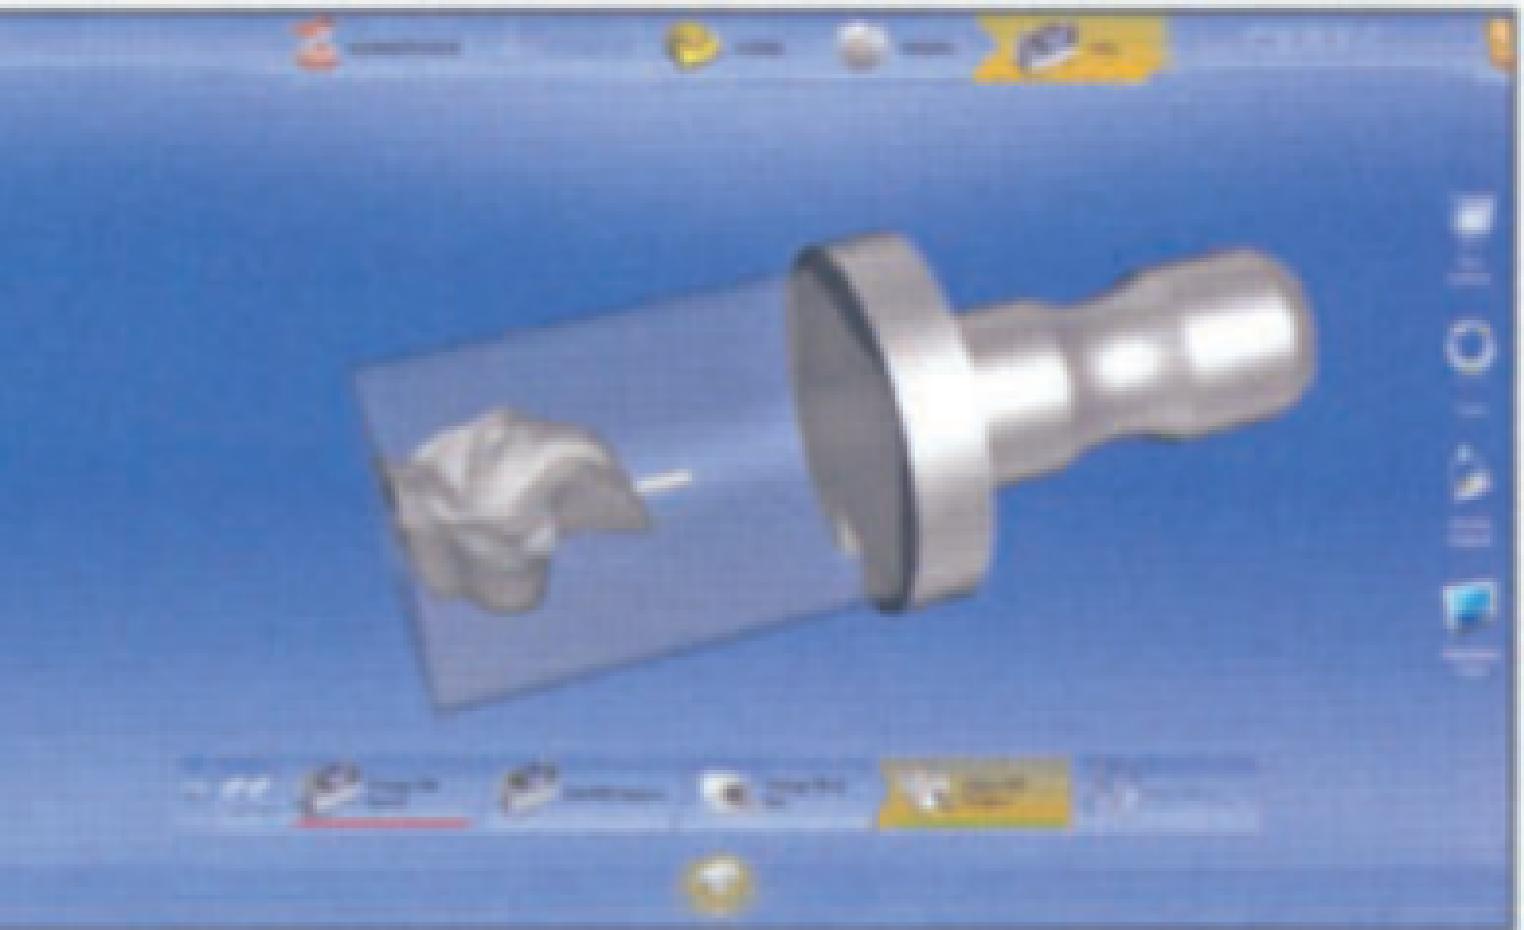


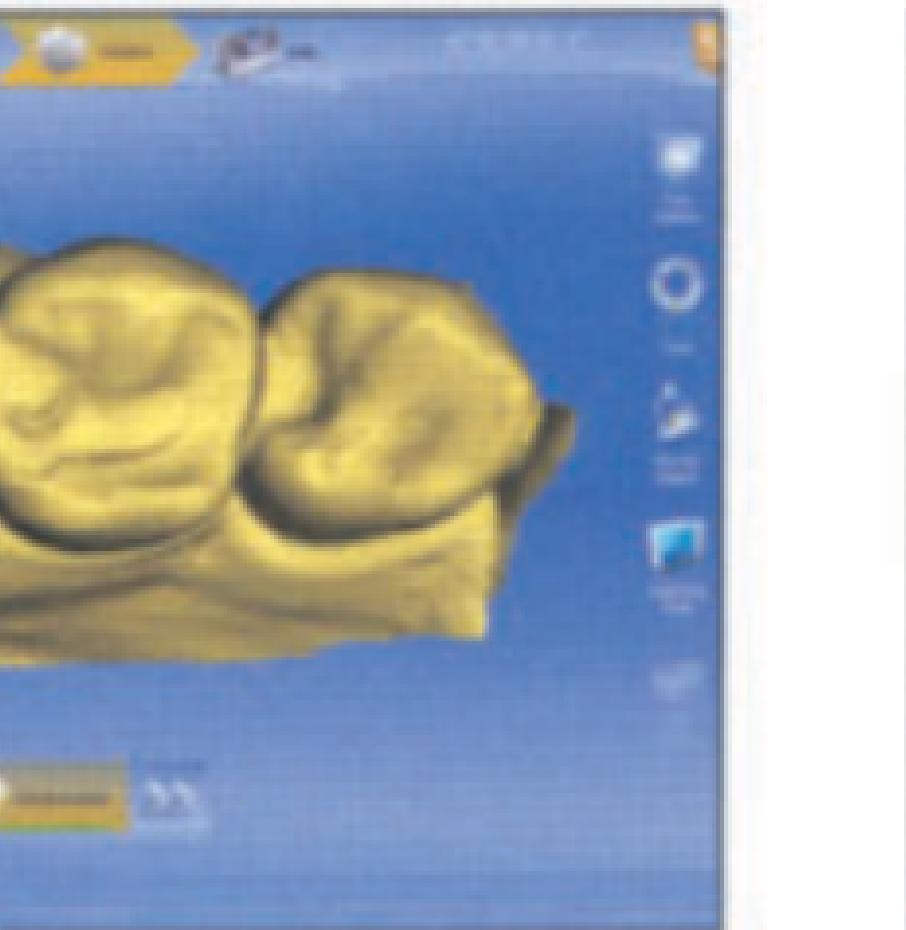


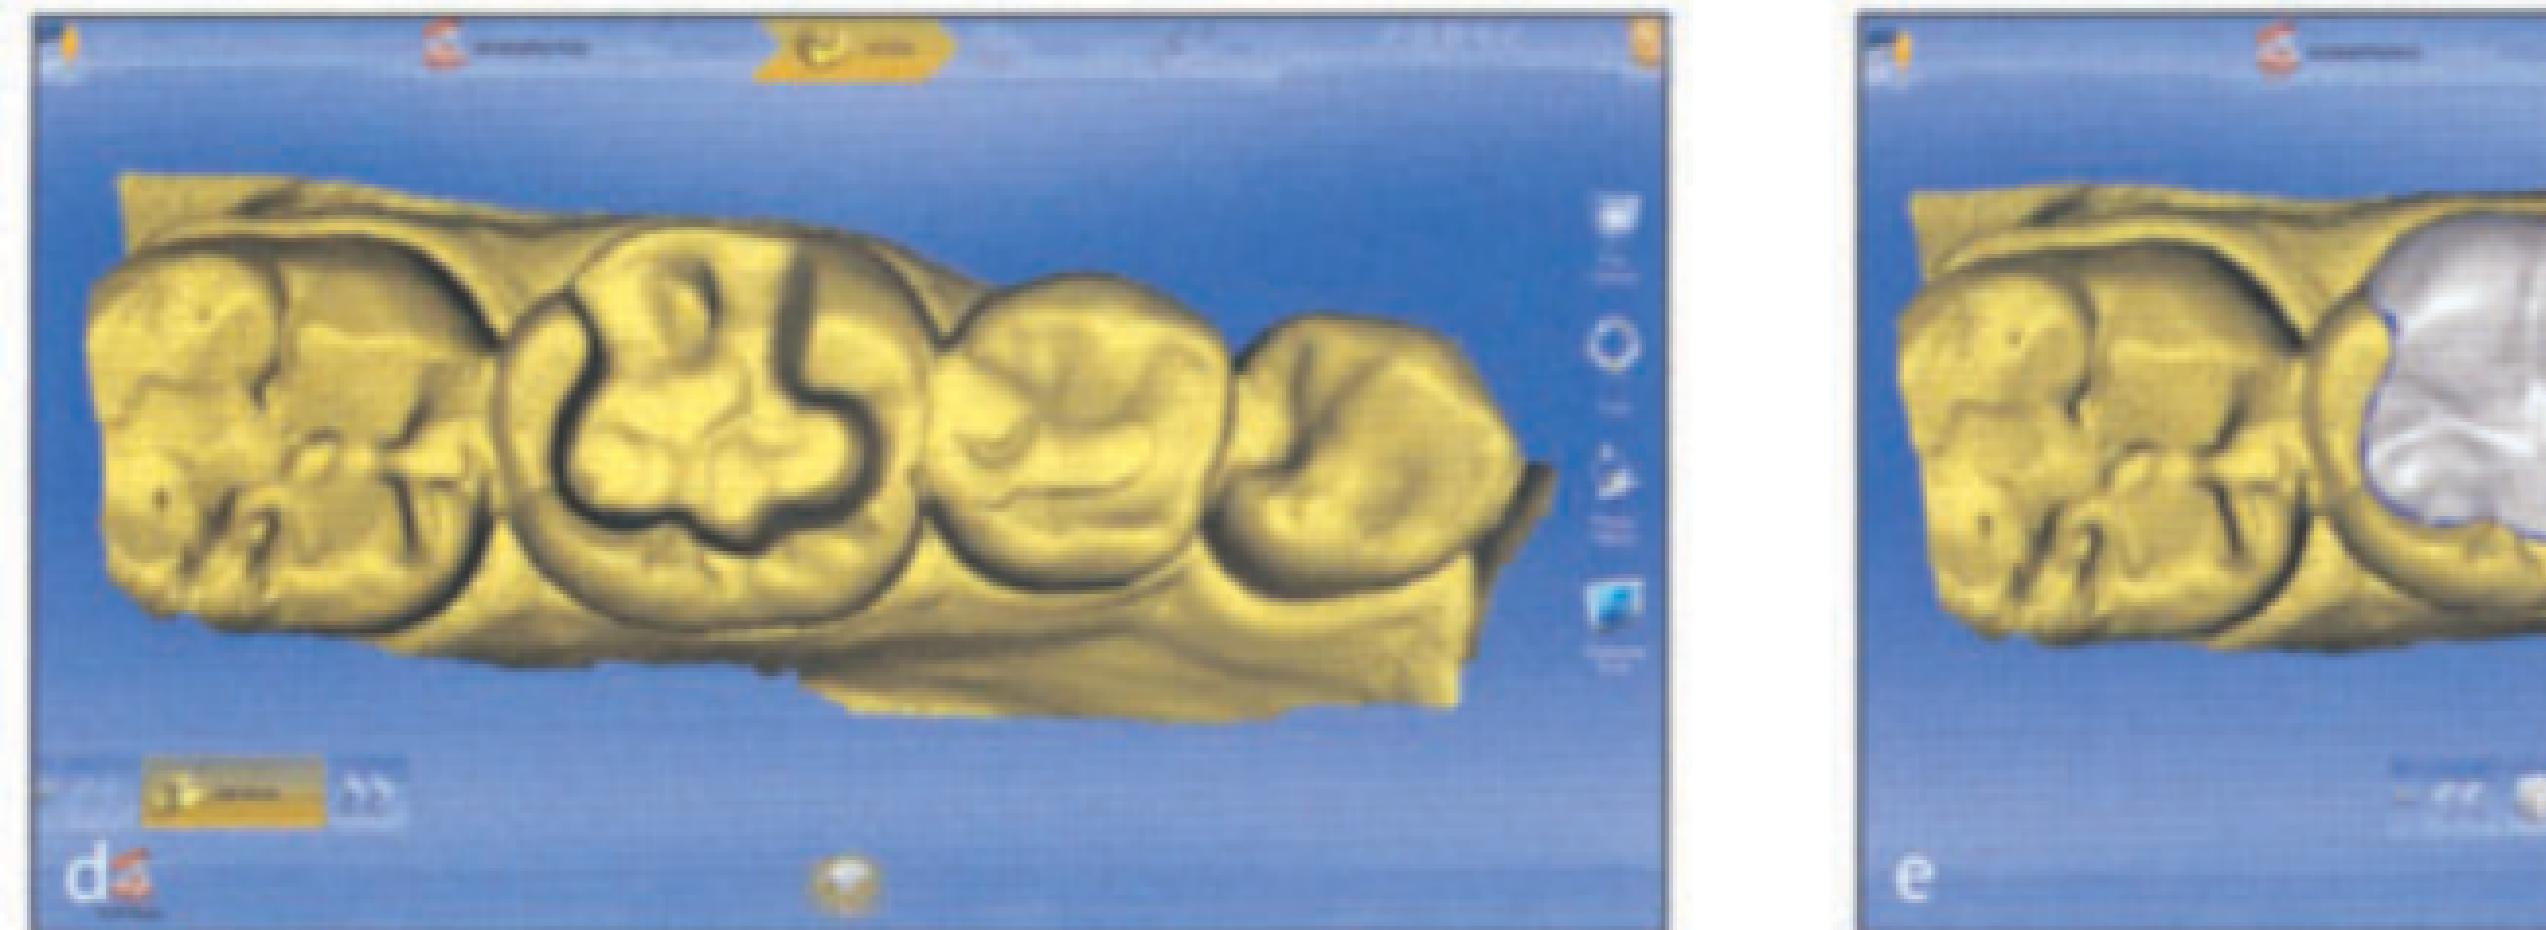



a






b

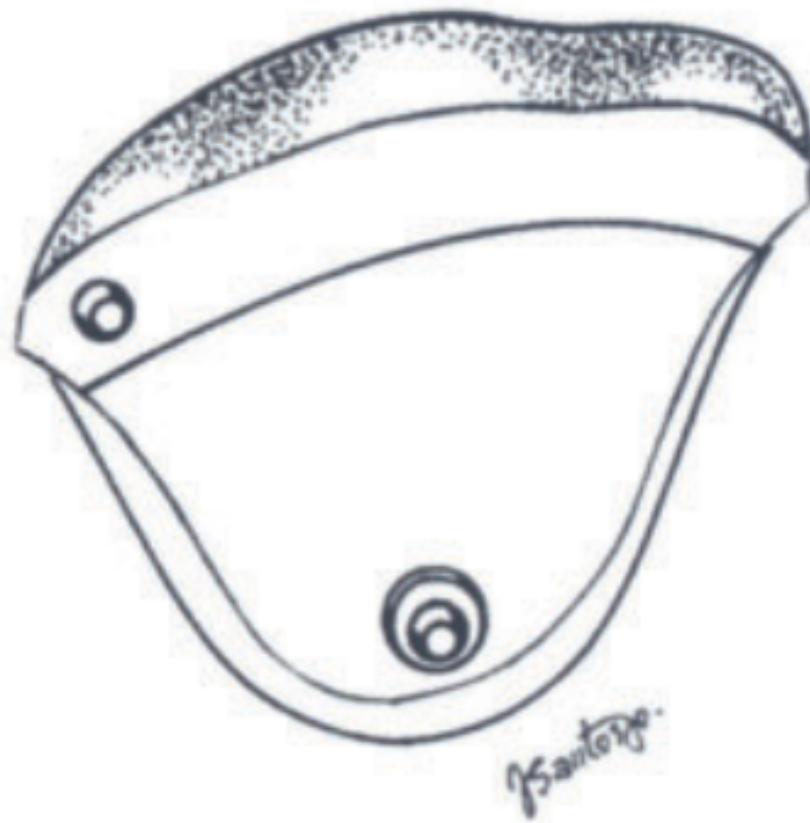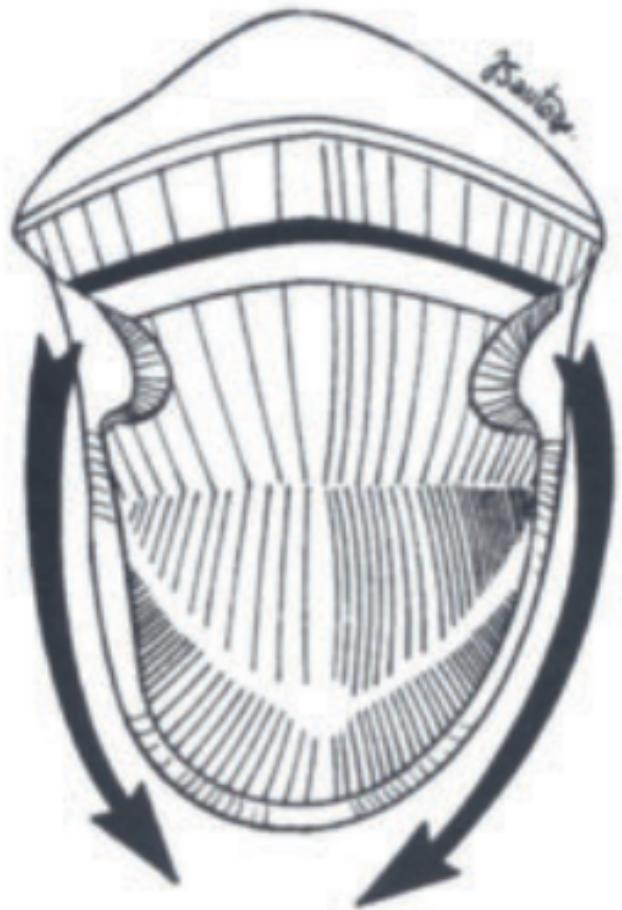

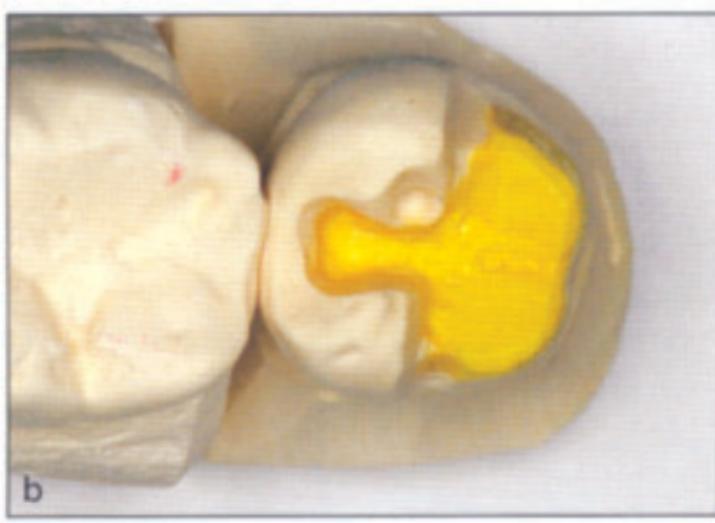

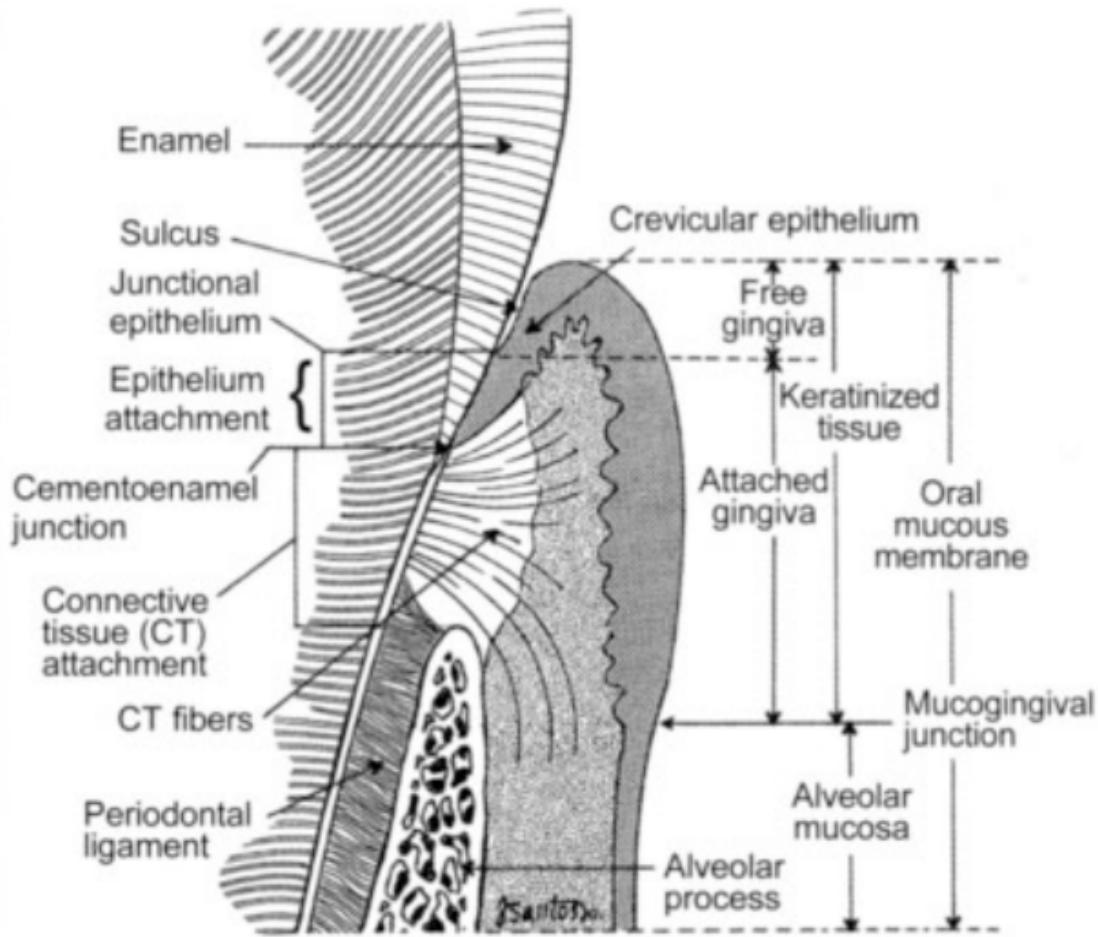

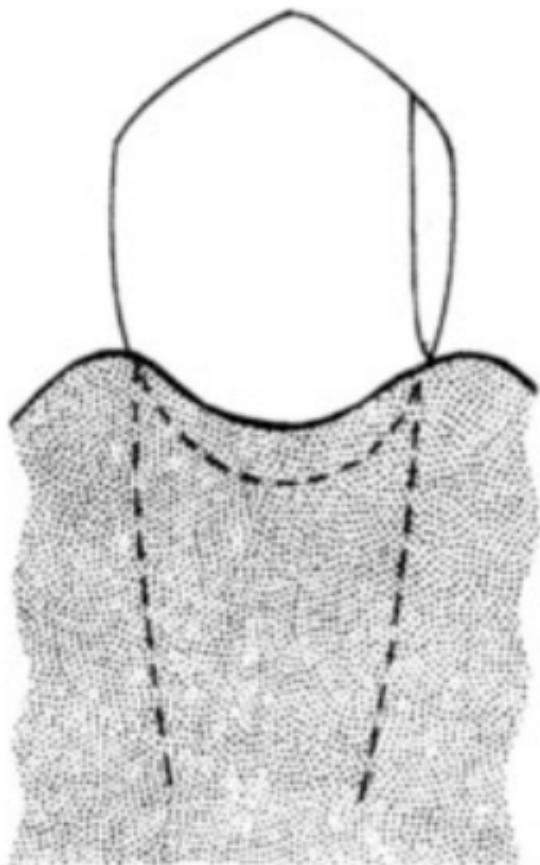

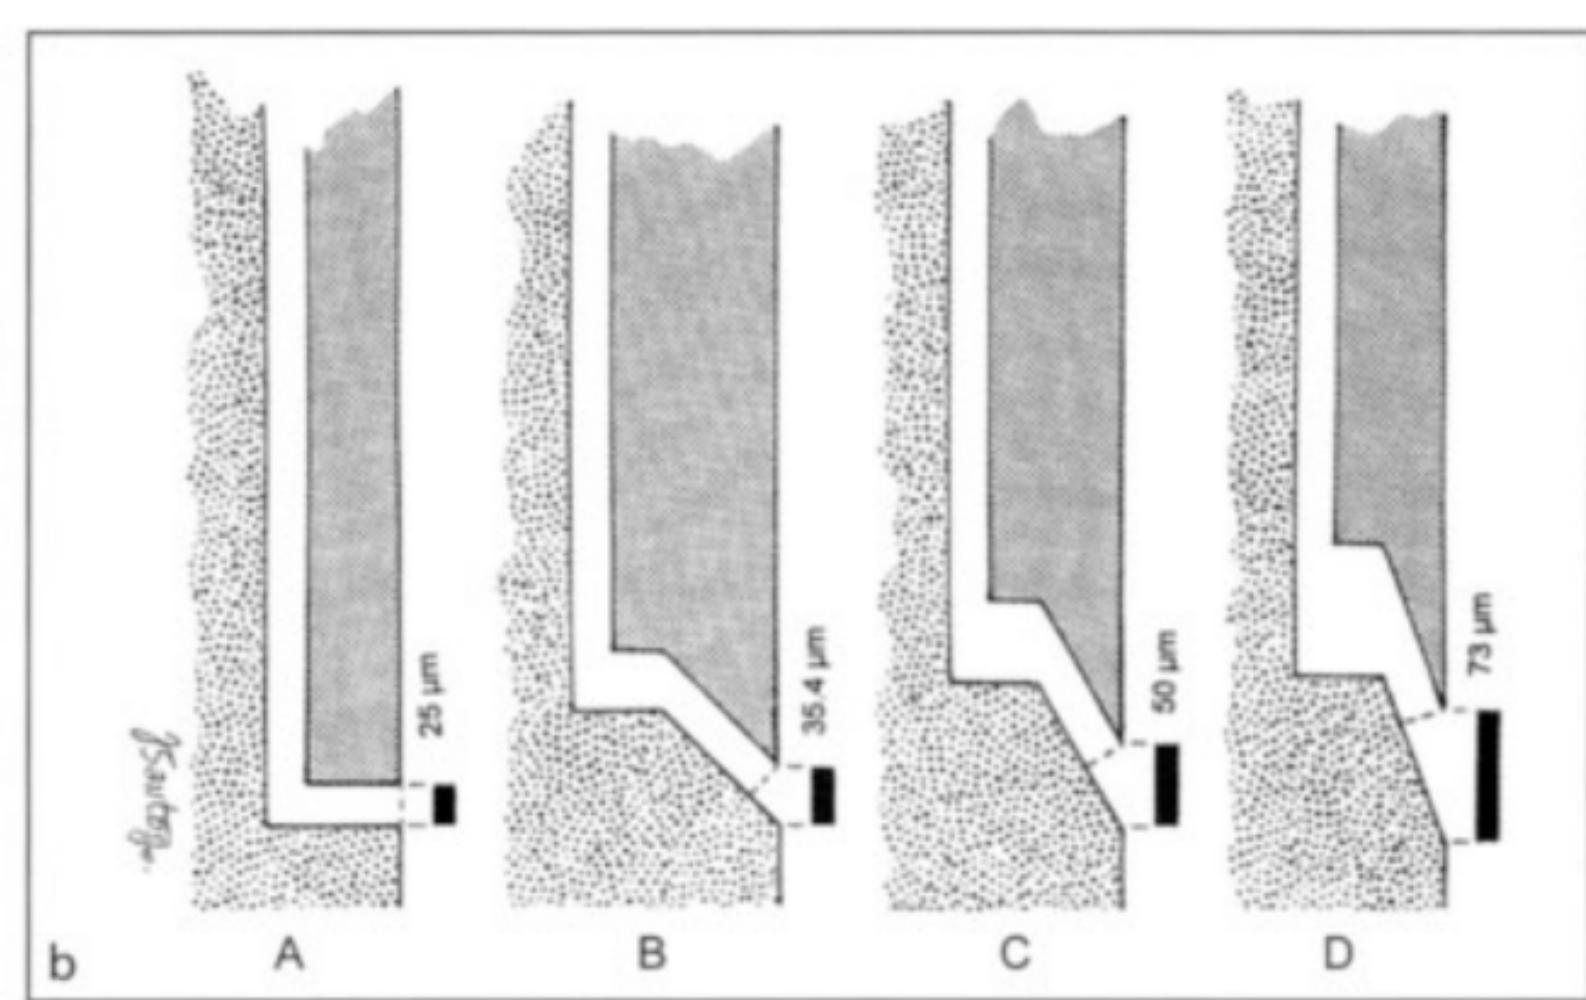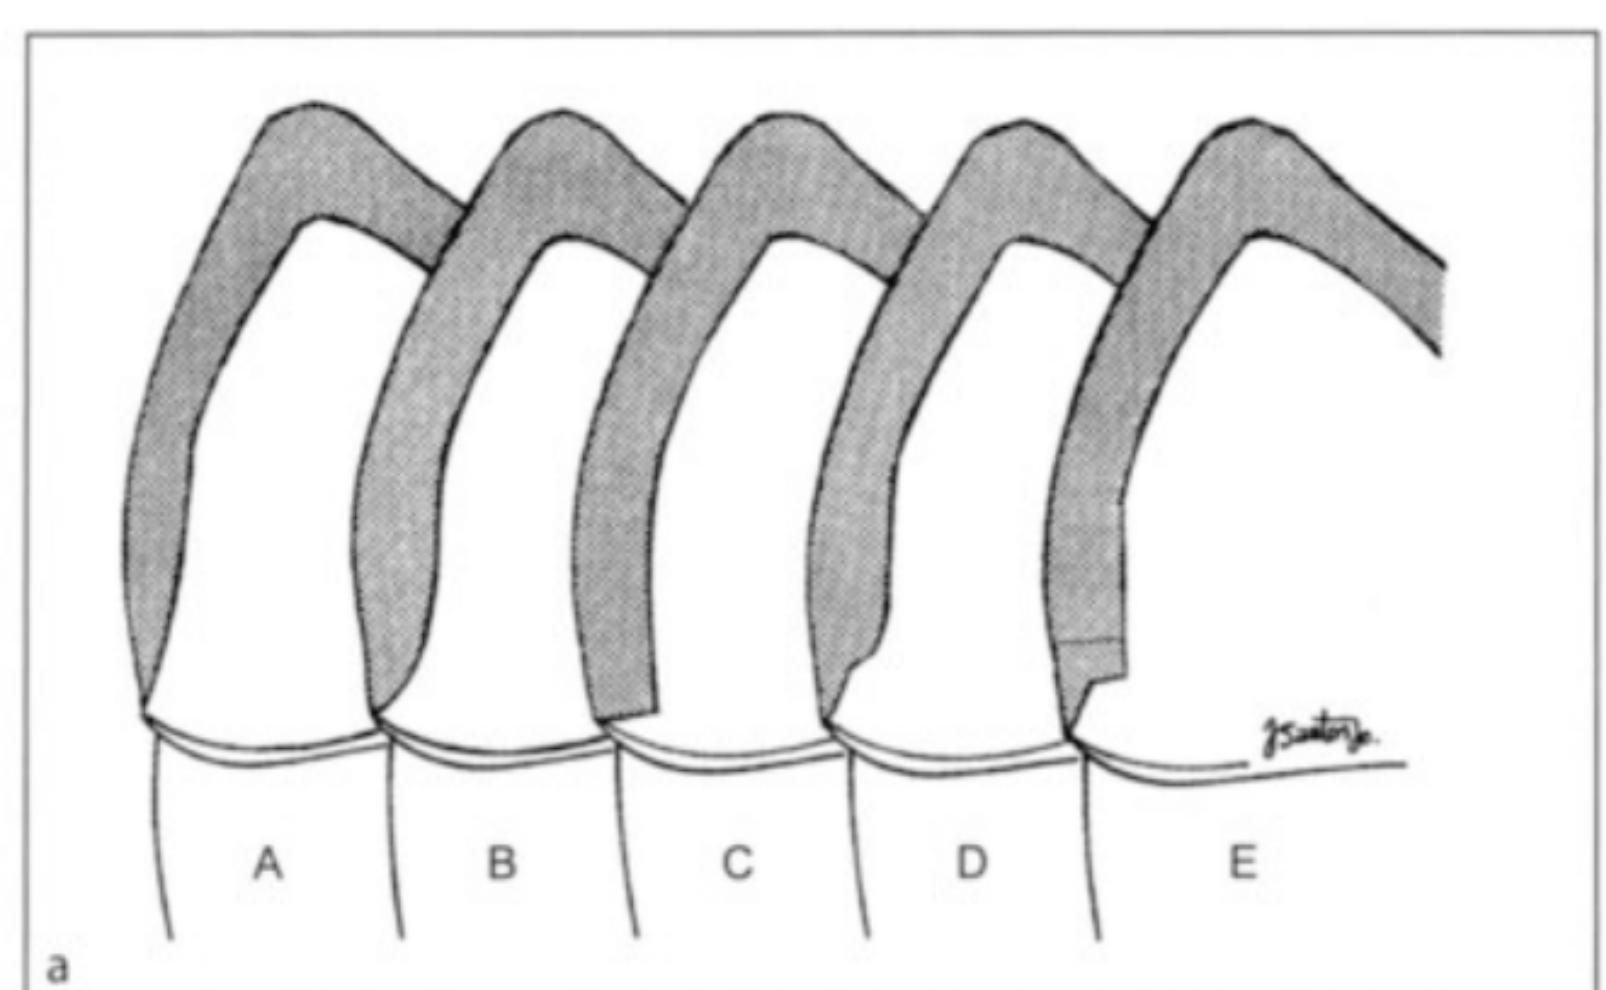







a




b



c



d

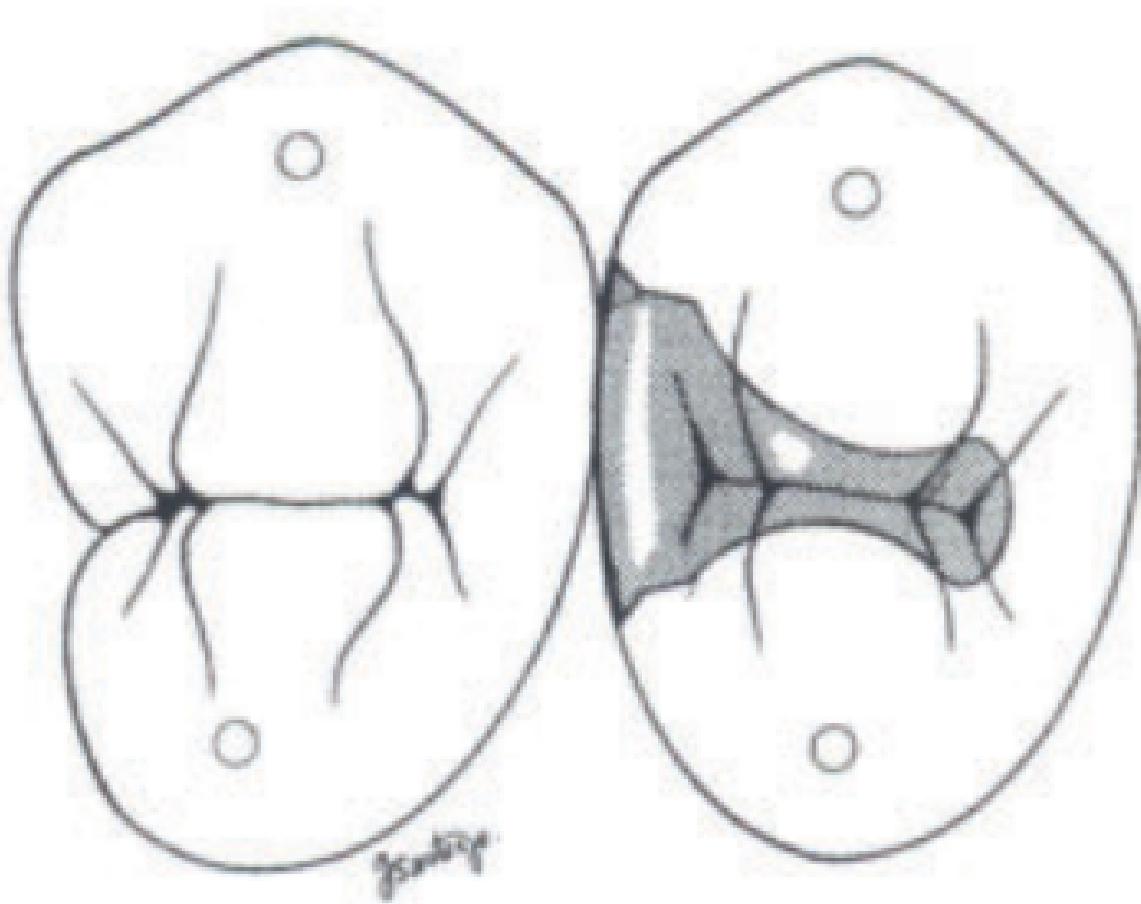








a




b

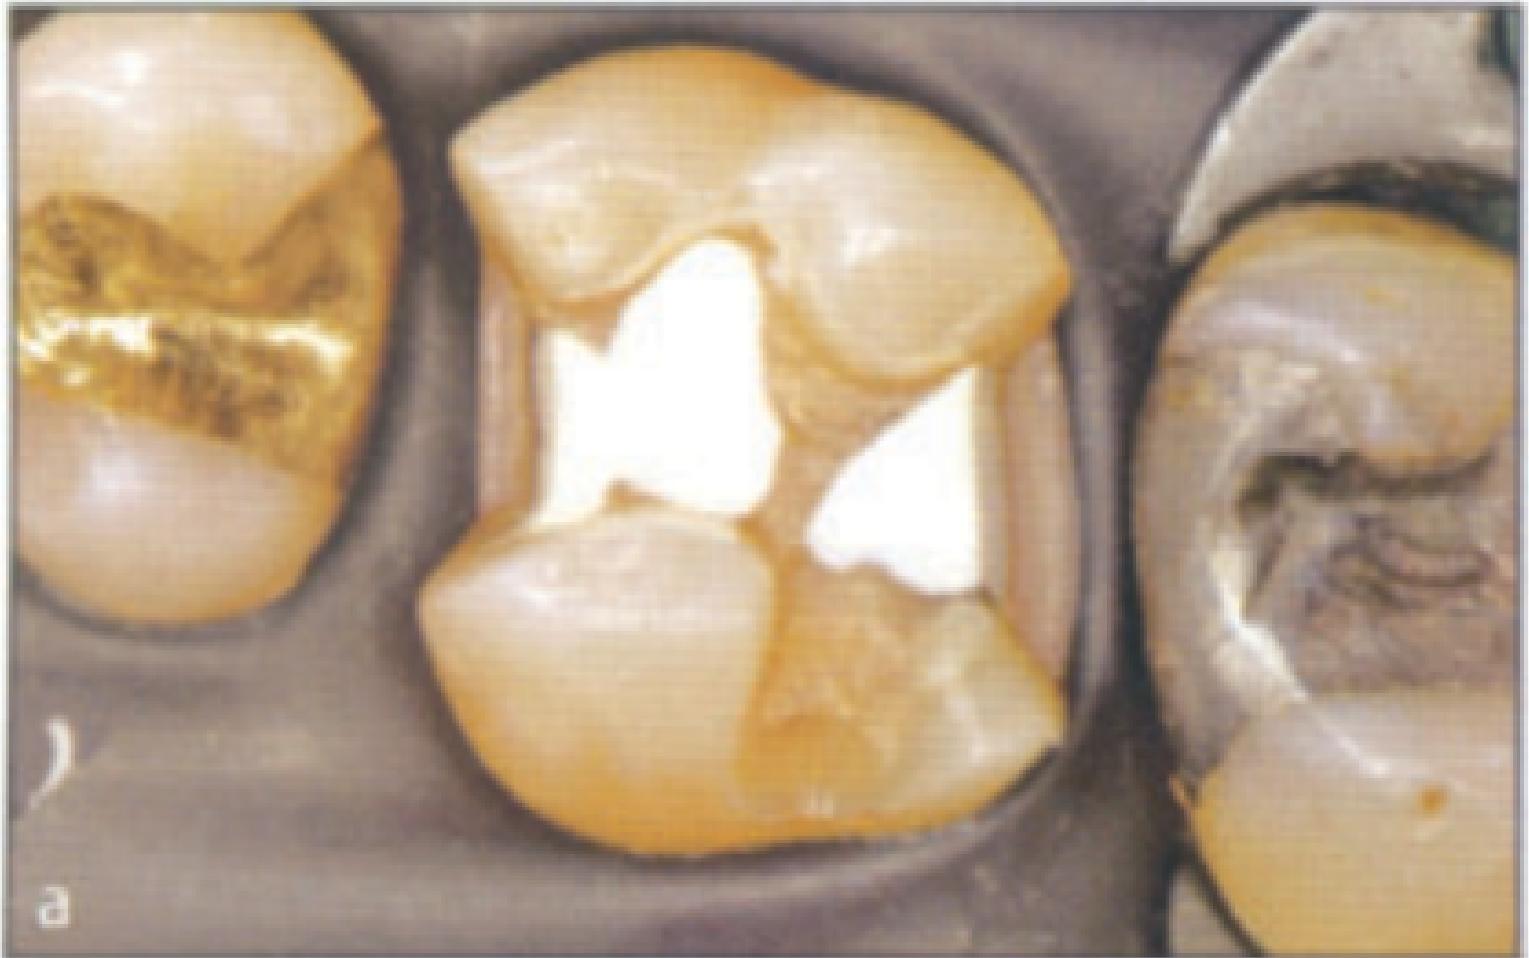


a





b



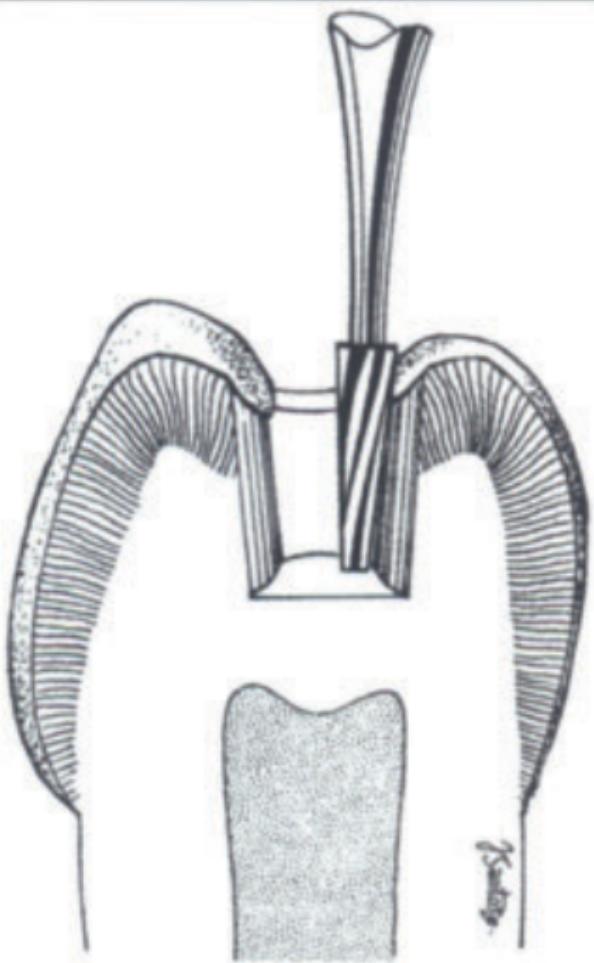




a



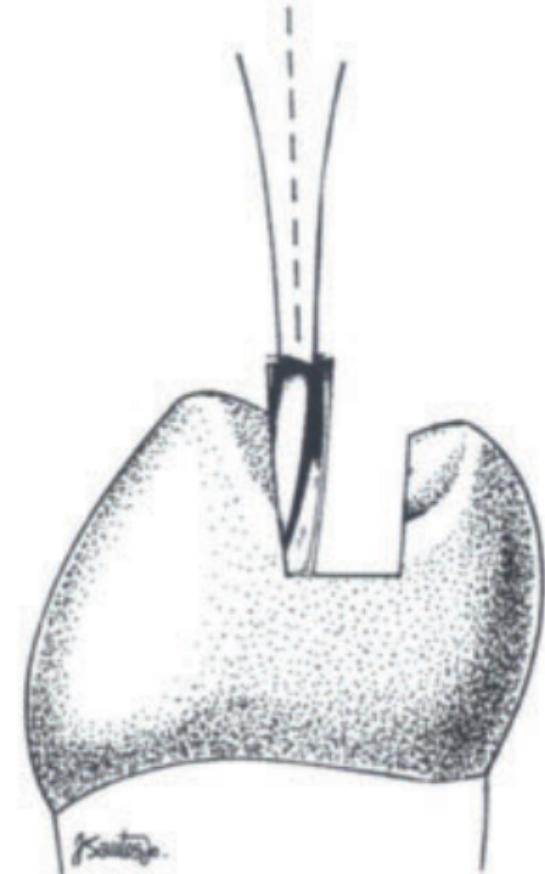



b

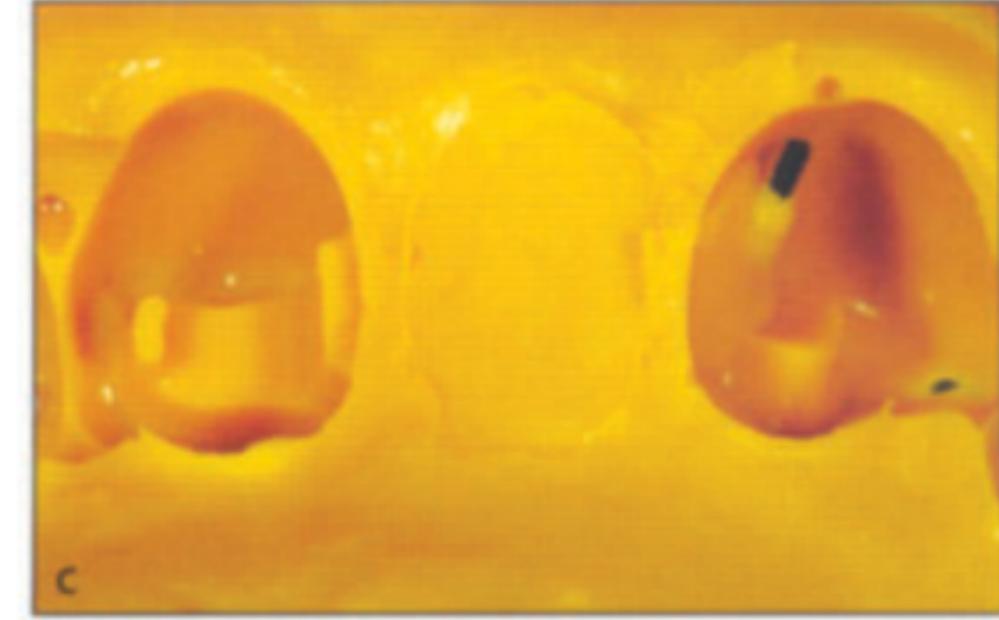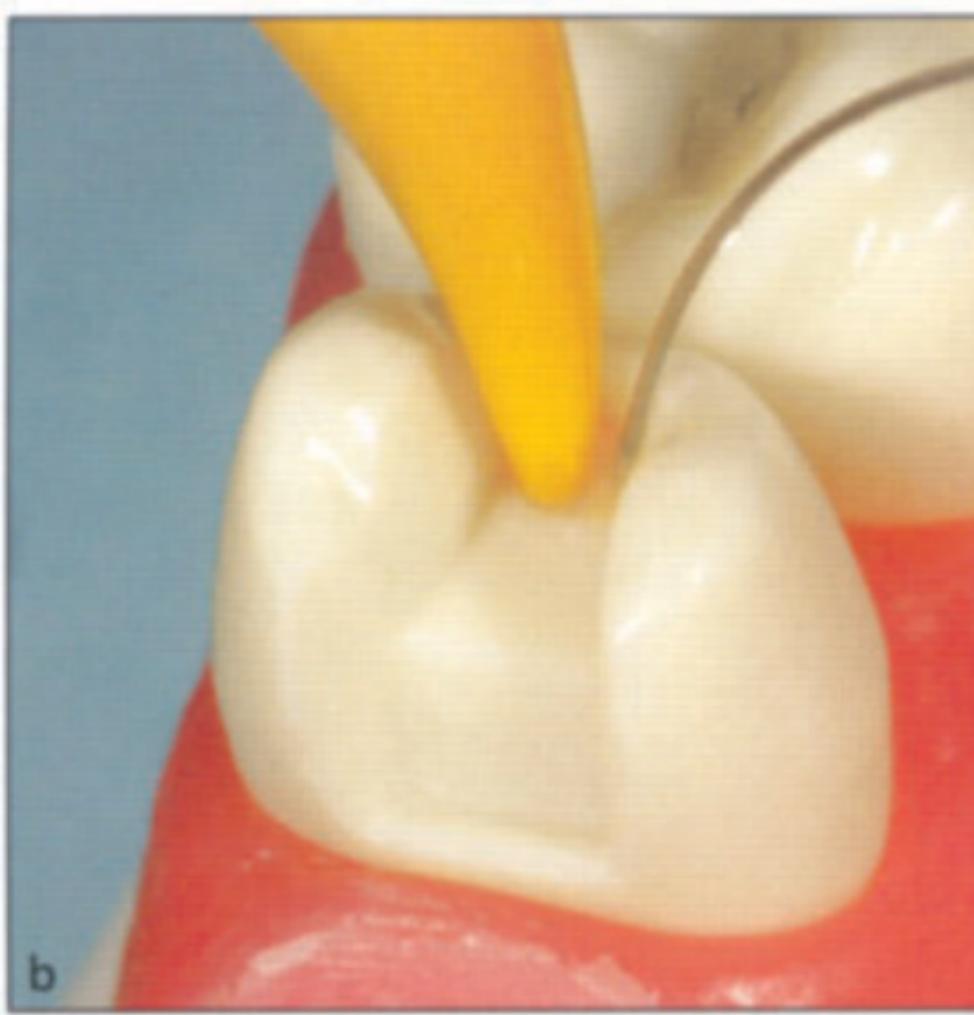

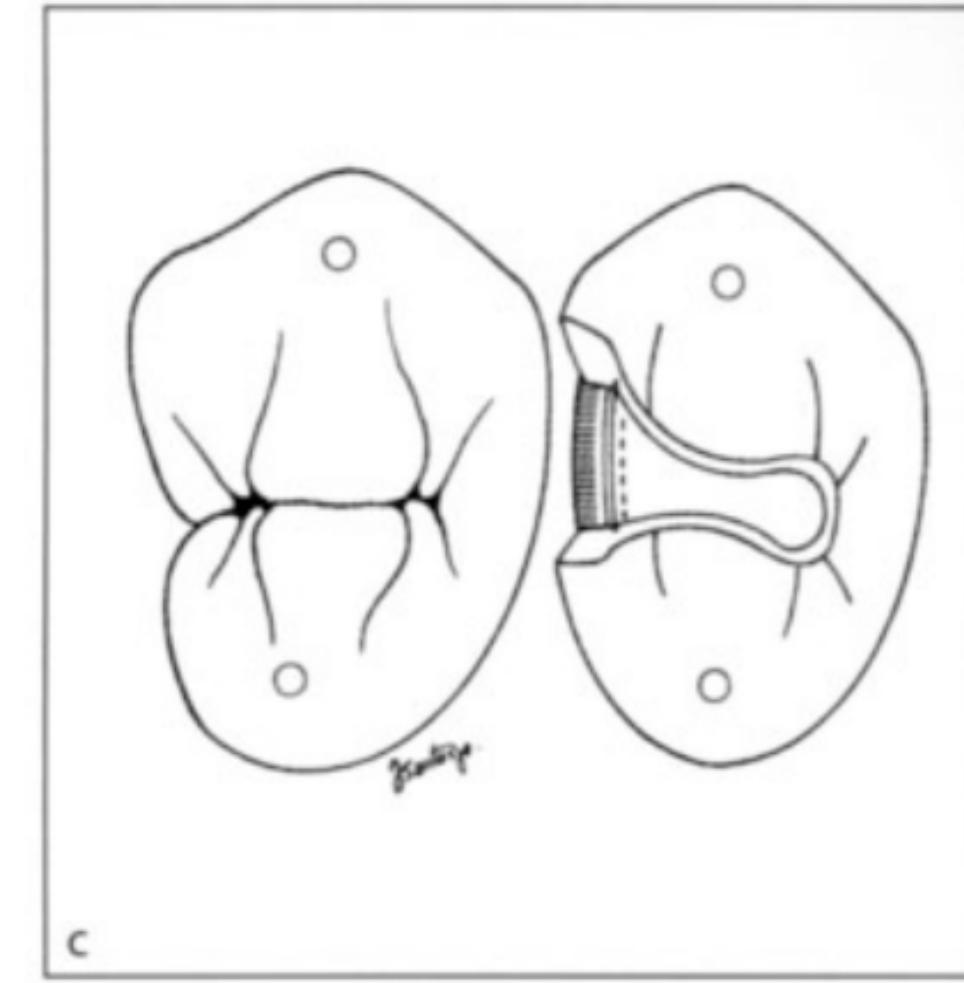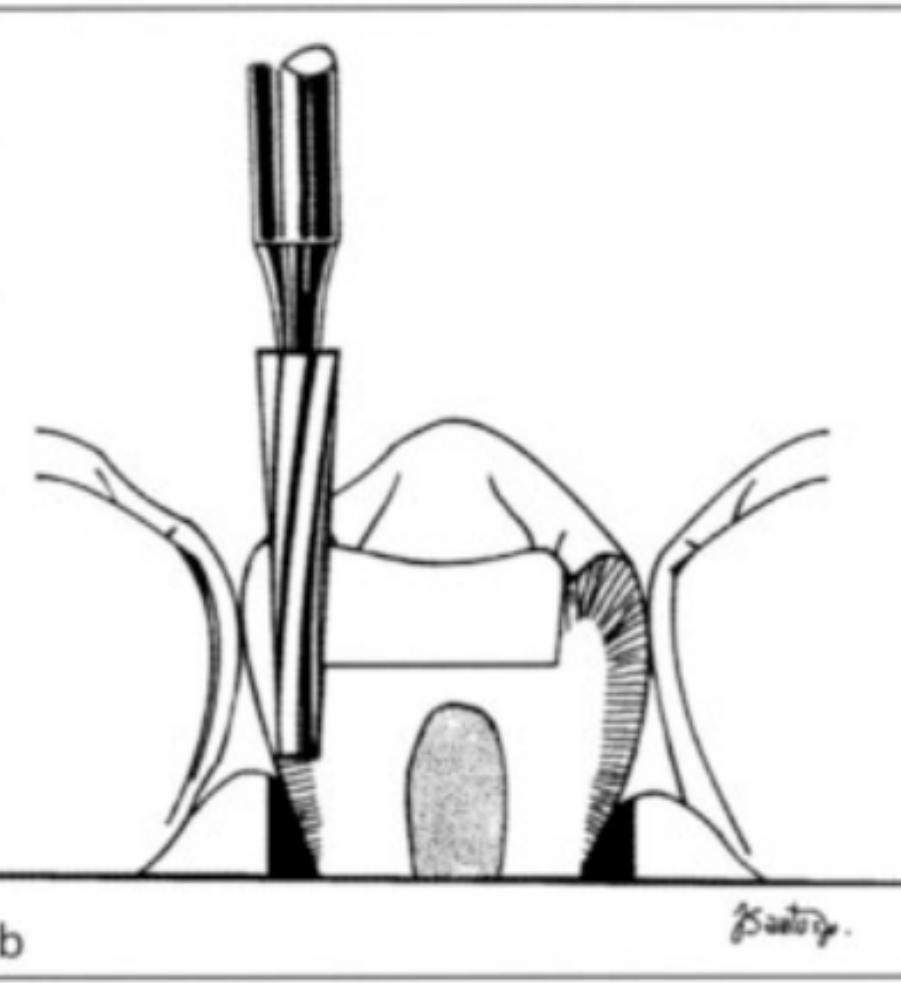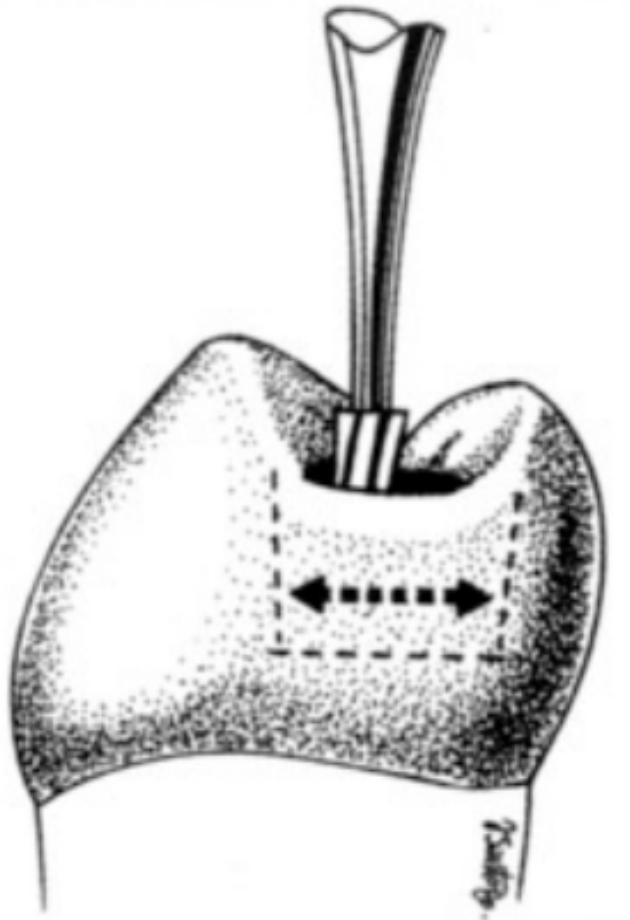


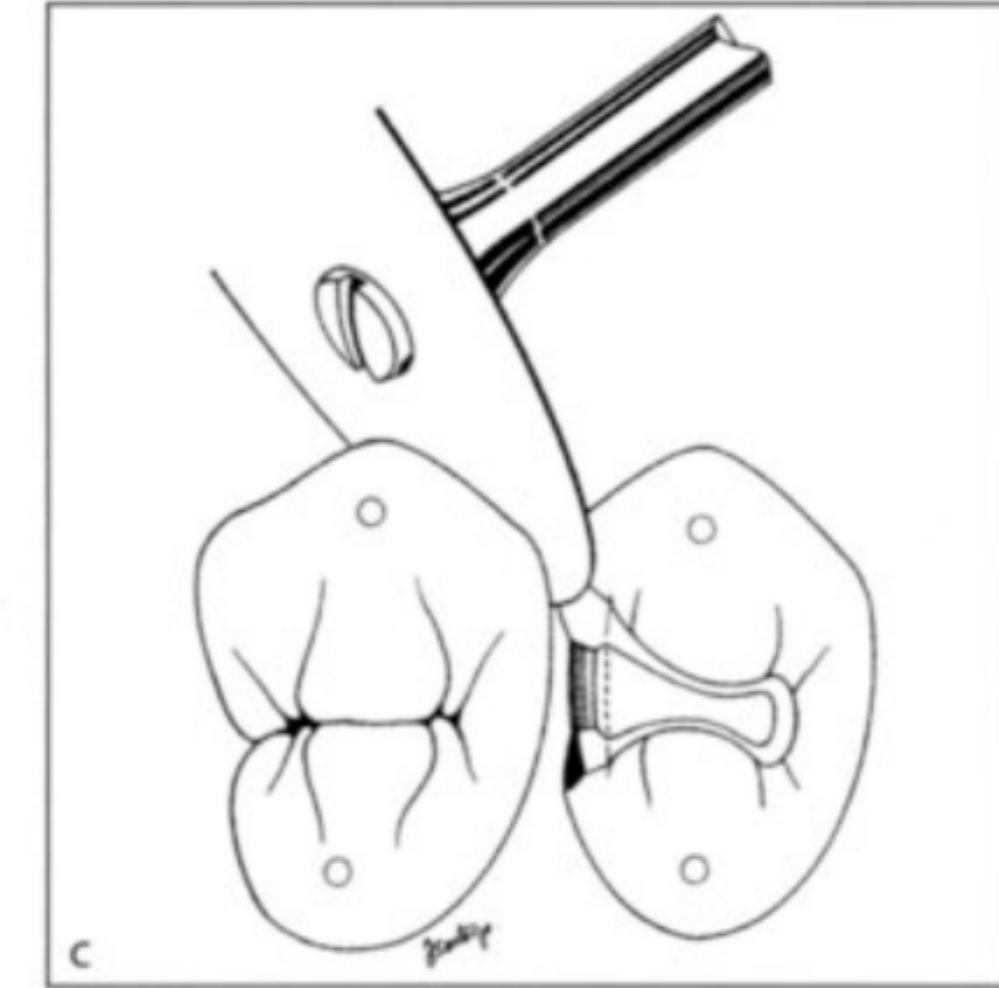
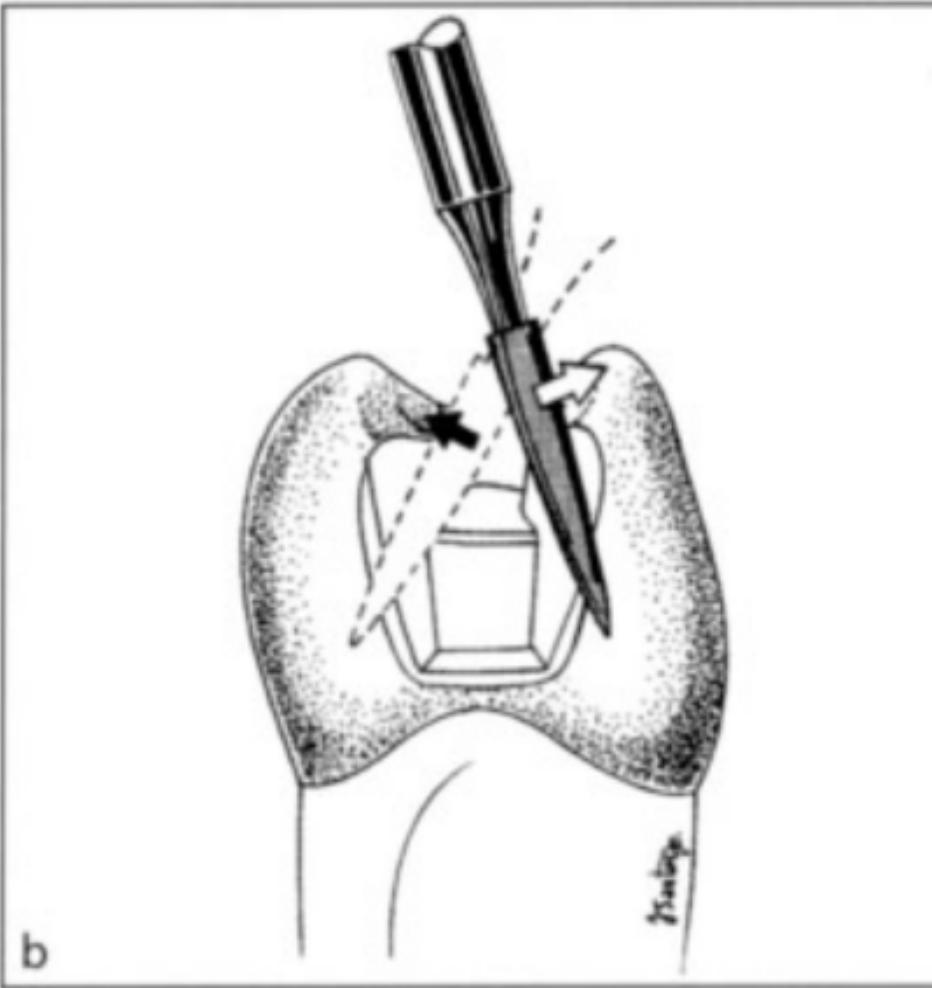


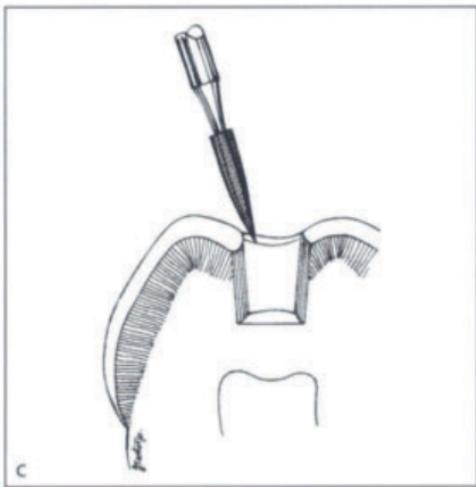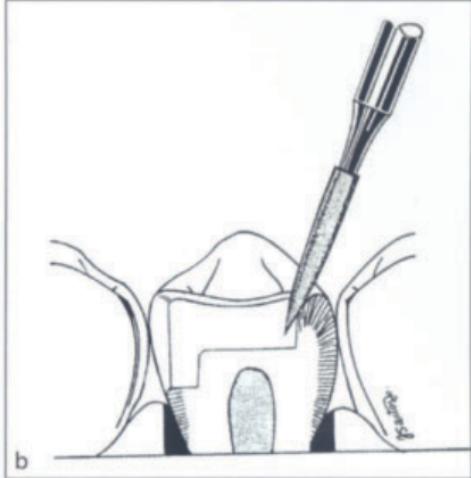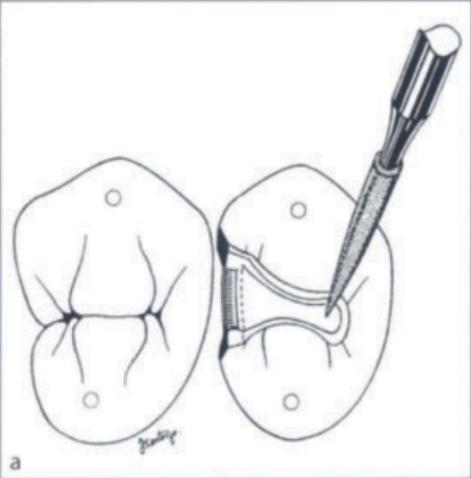


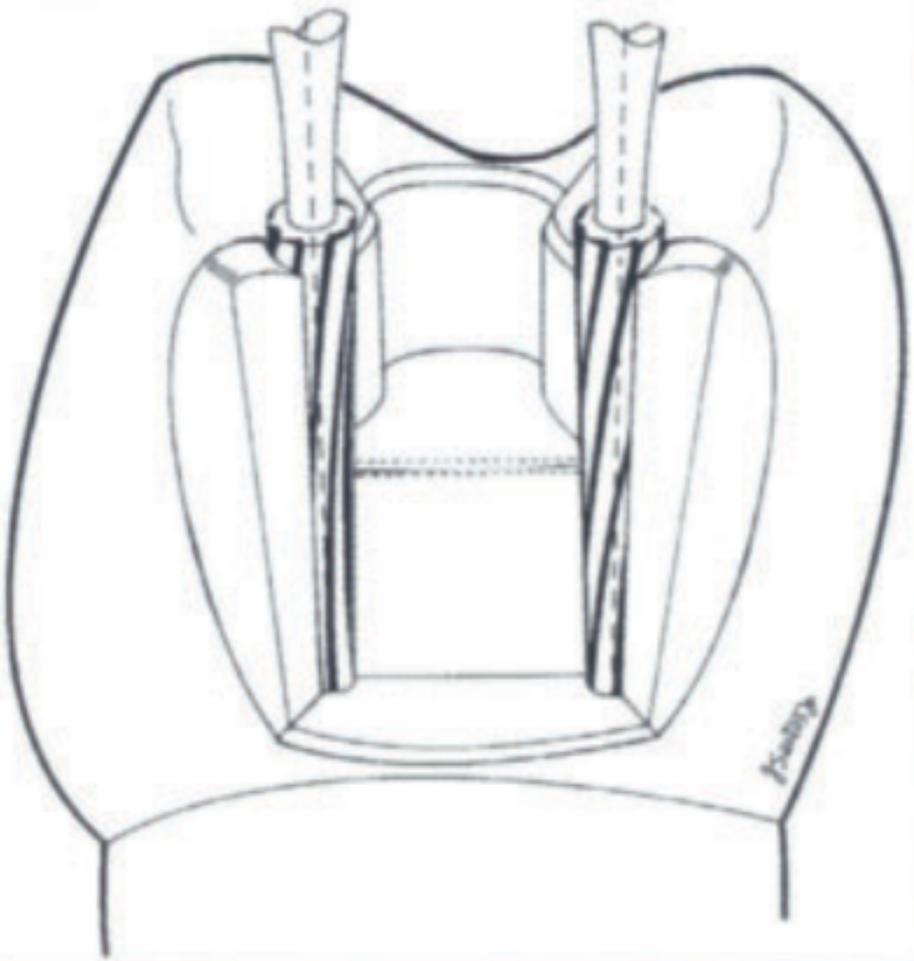




6-10 degrees

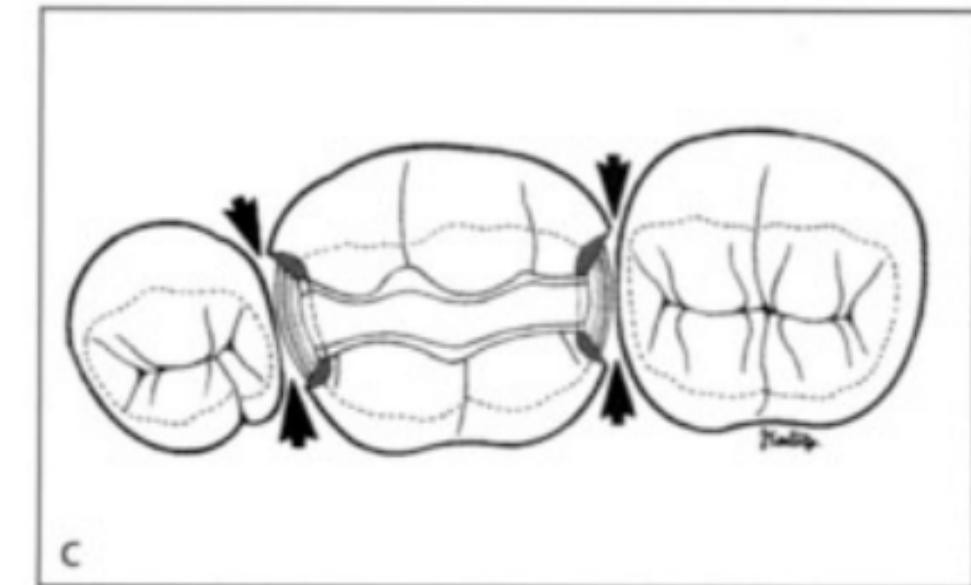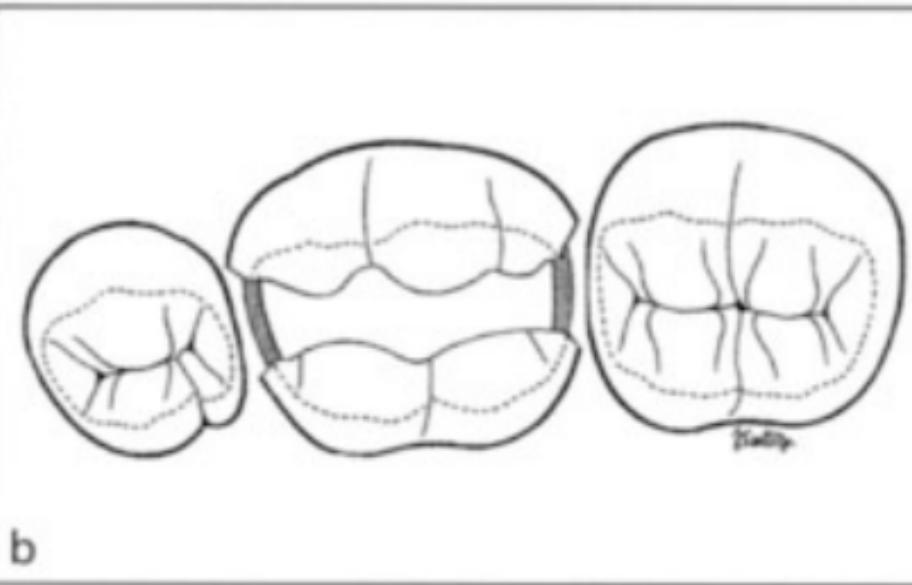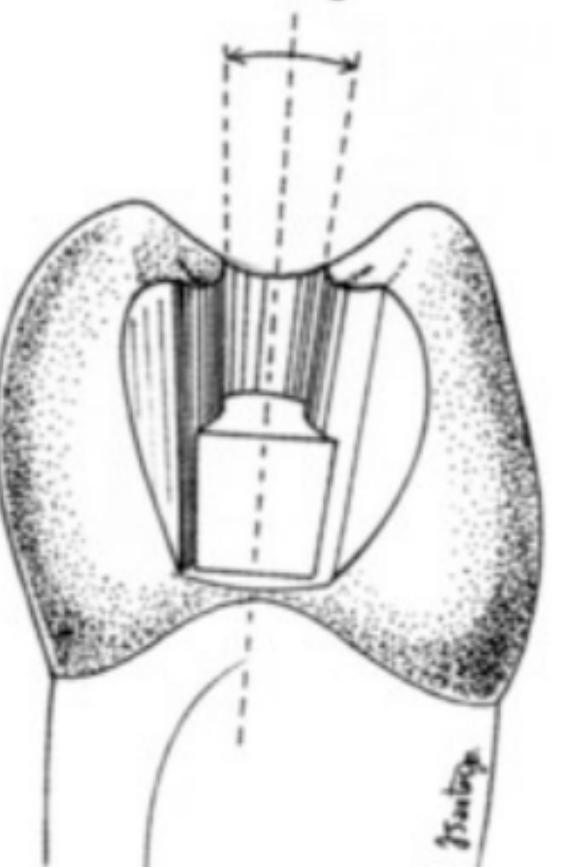


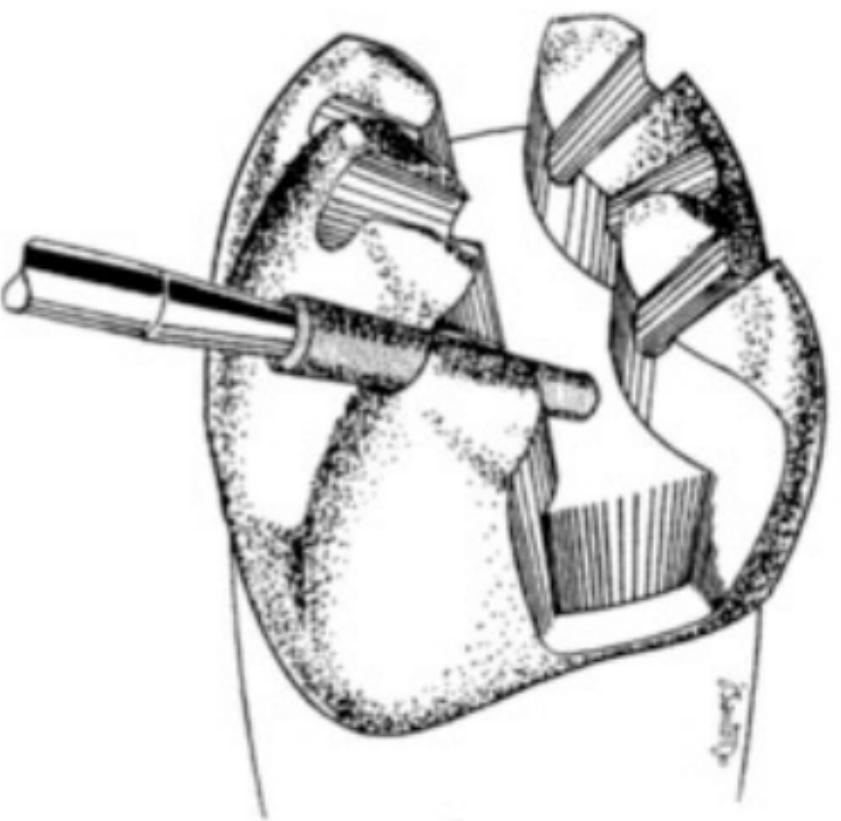


a

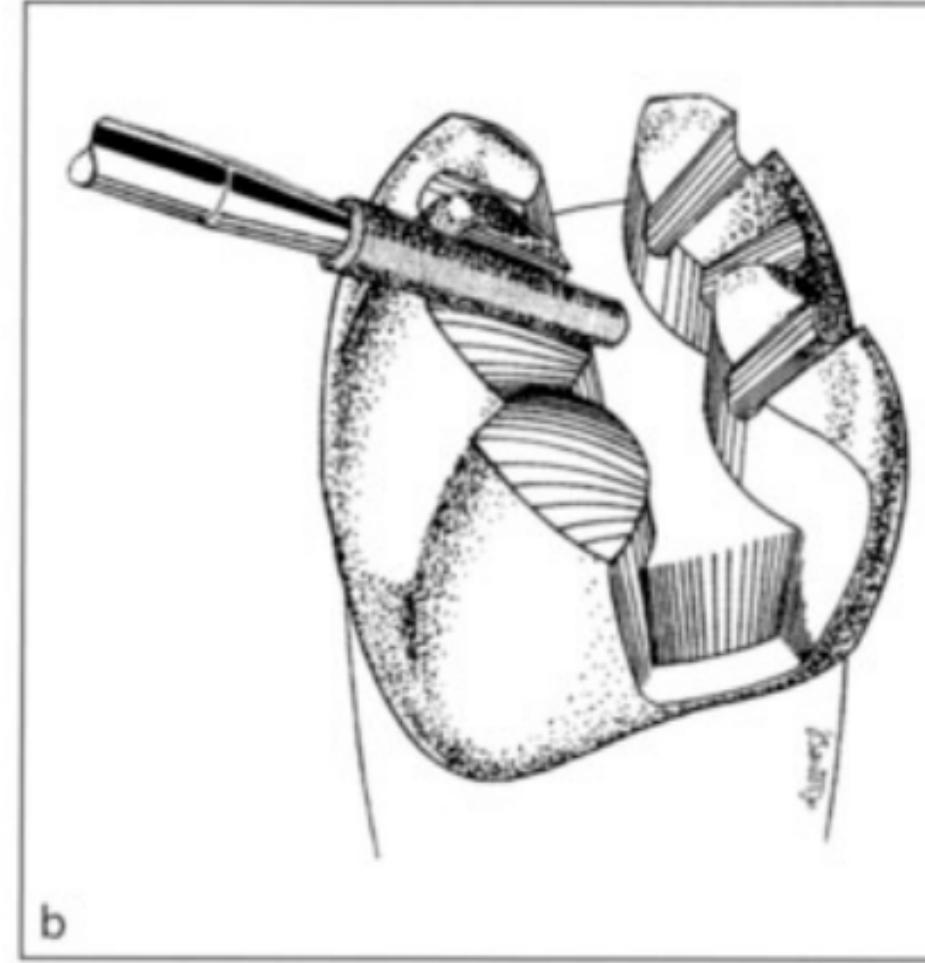



b

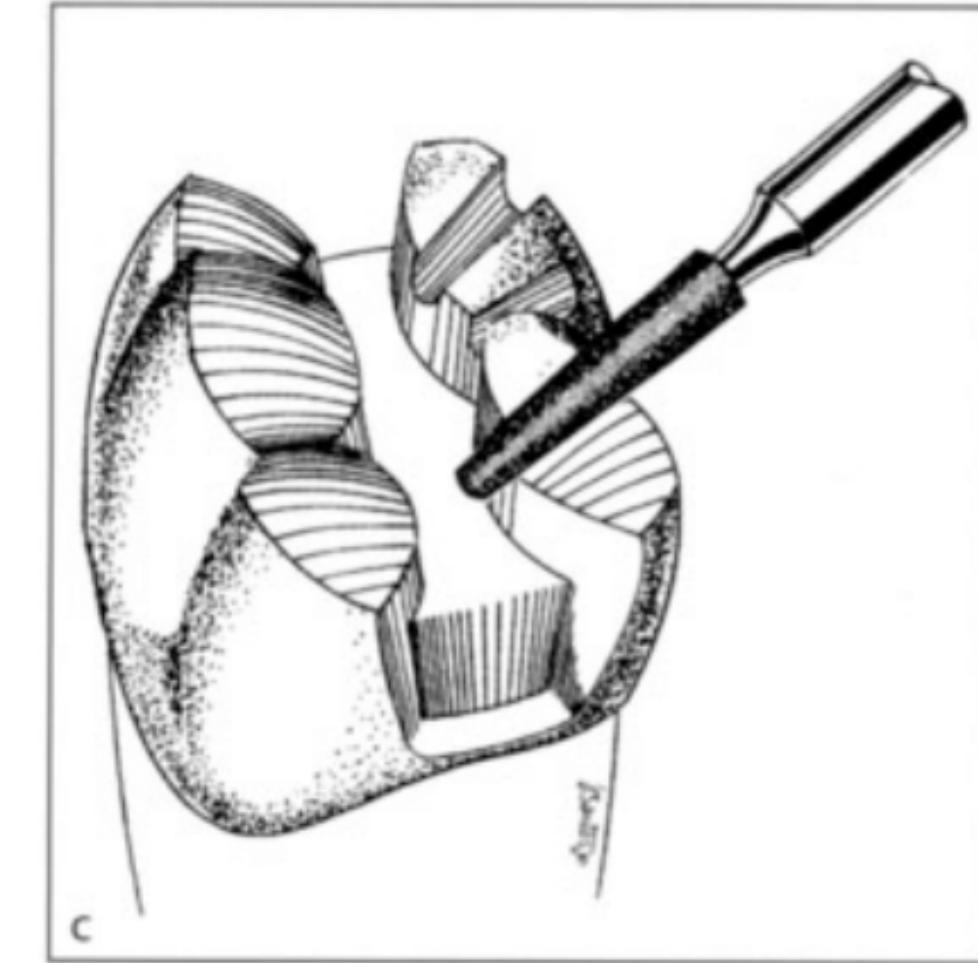



c


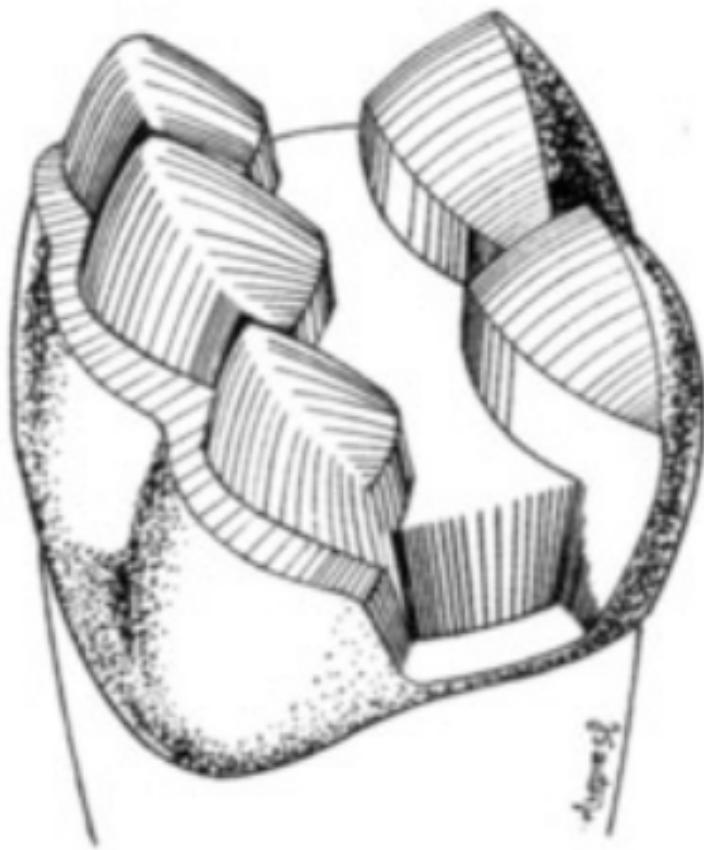


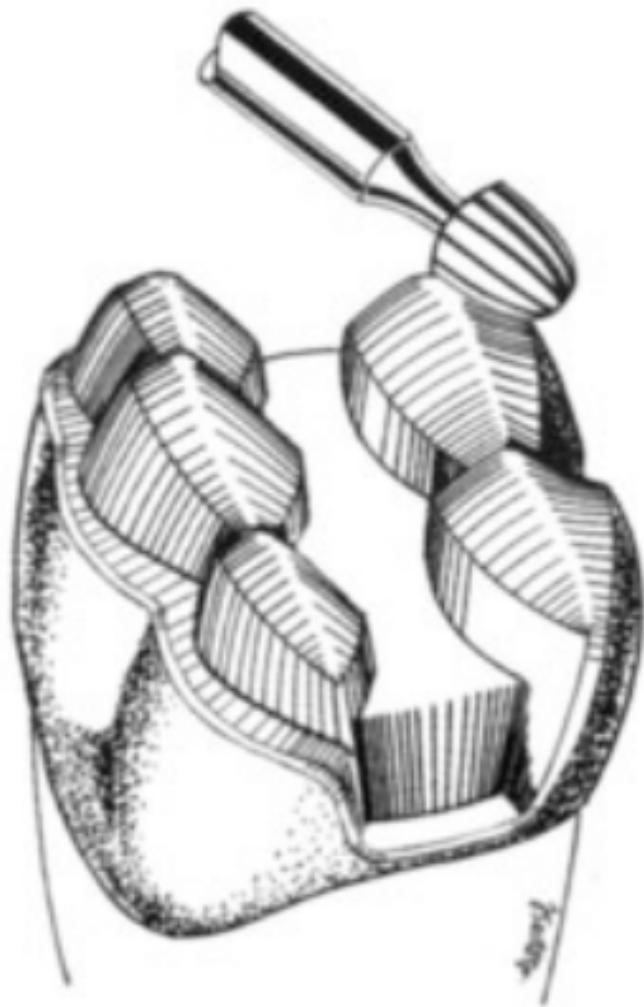


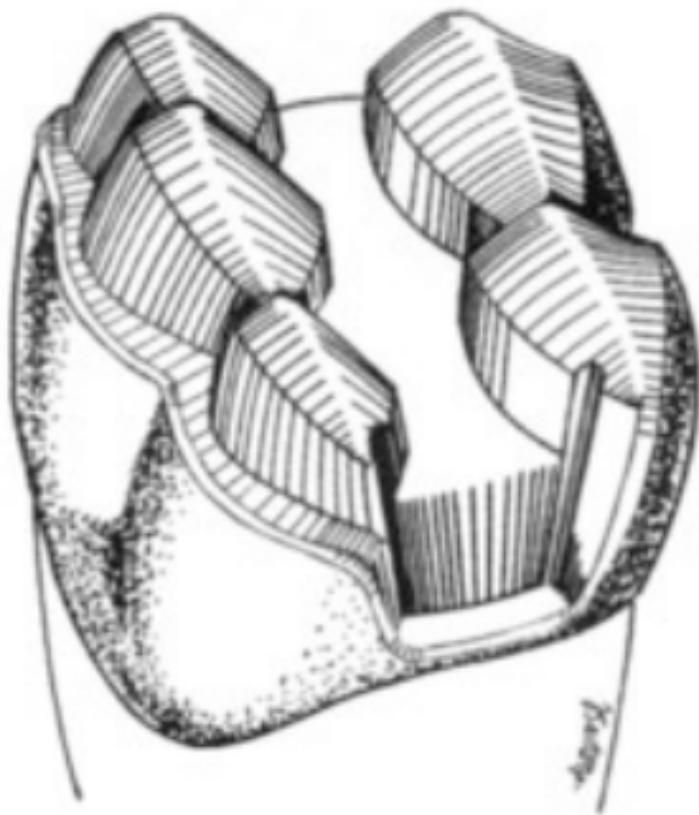


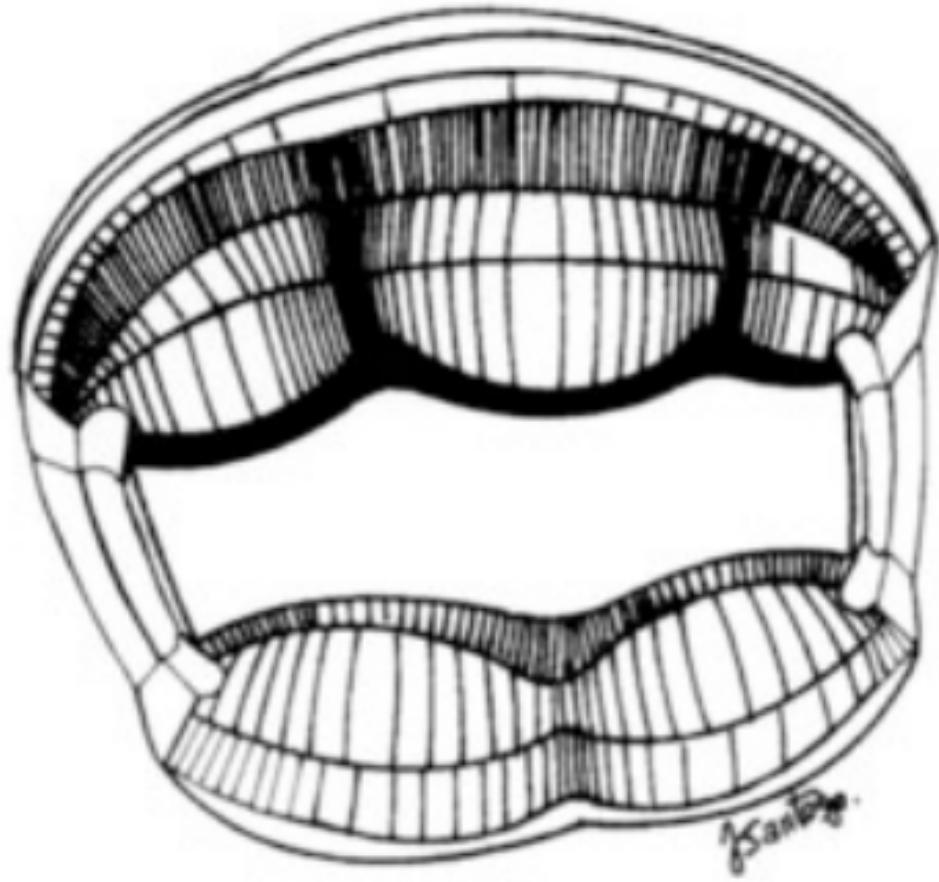


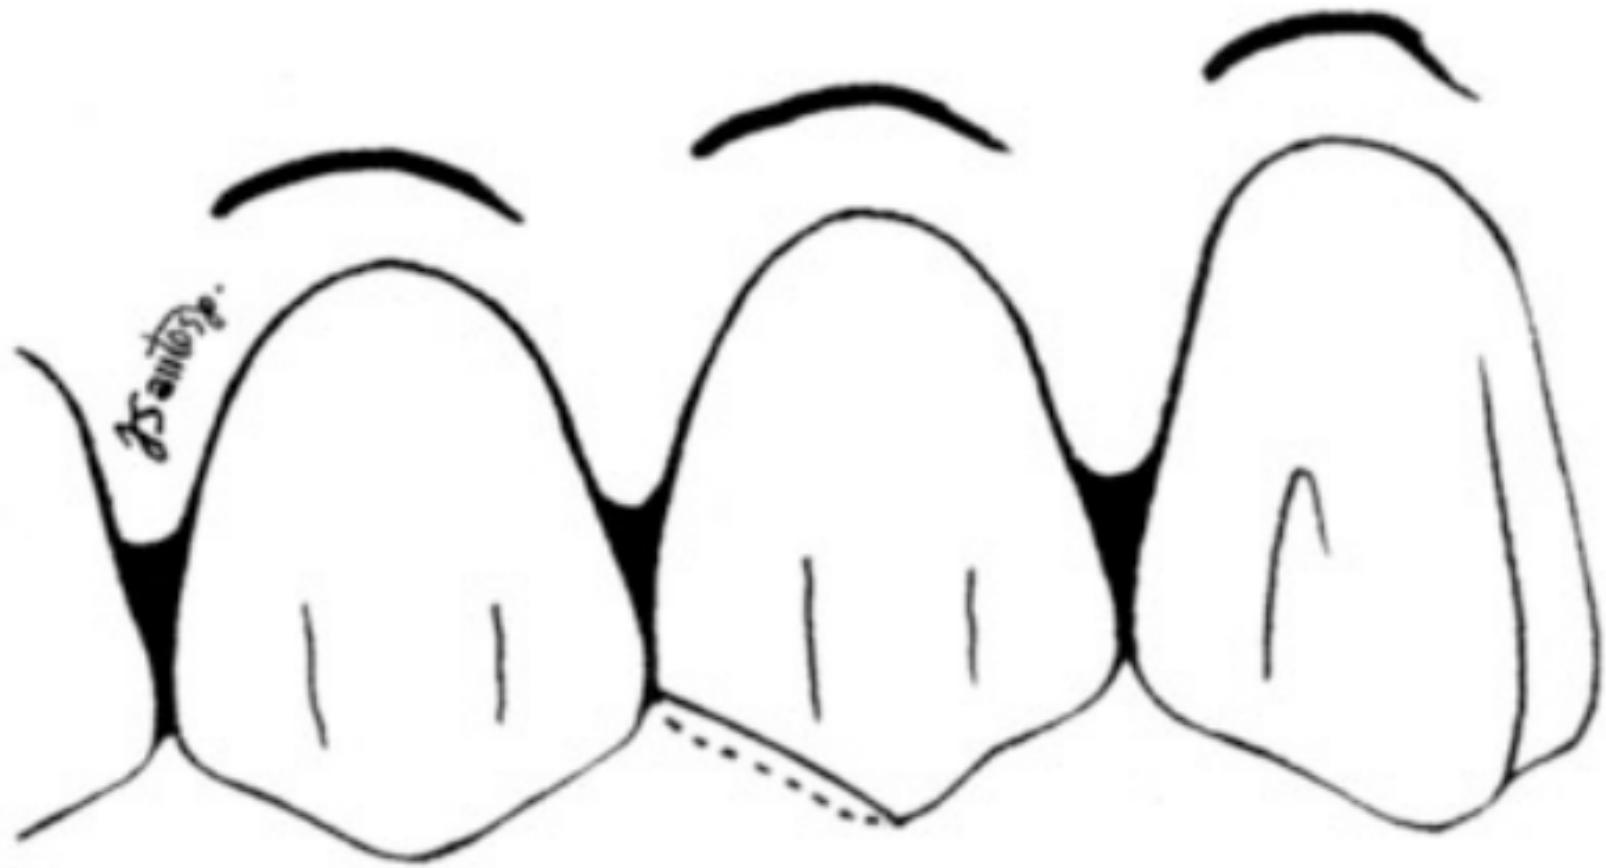

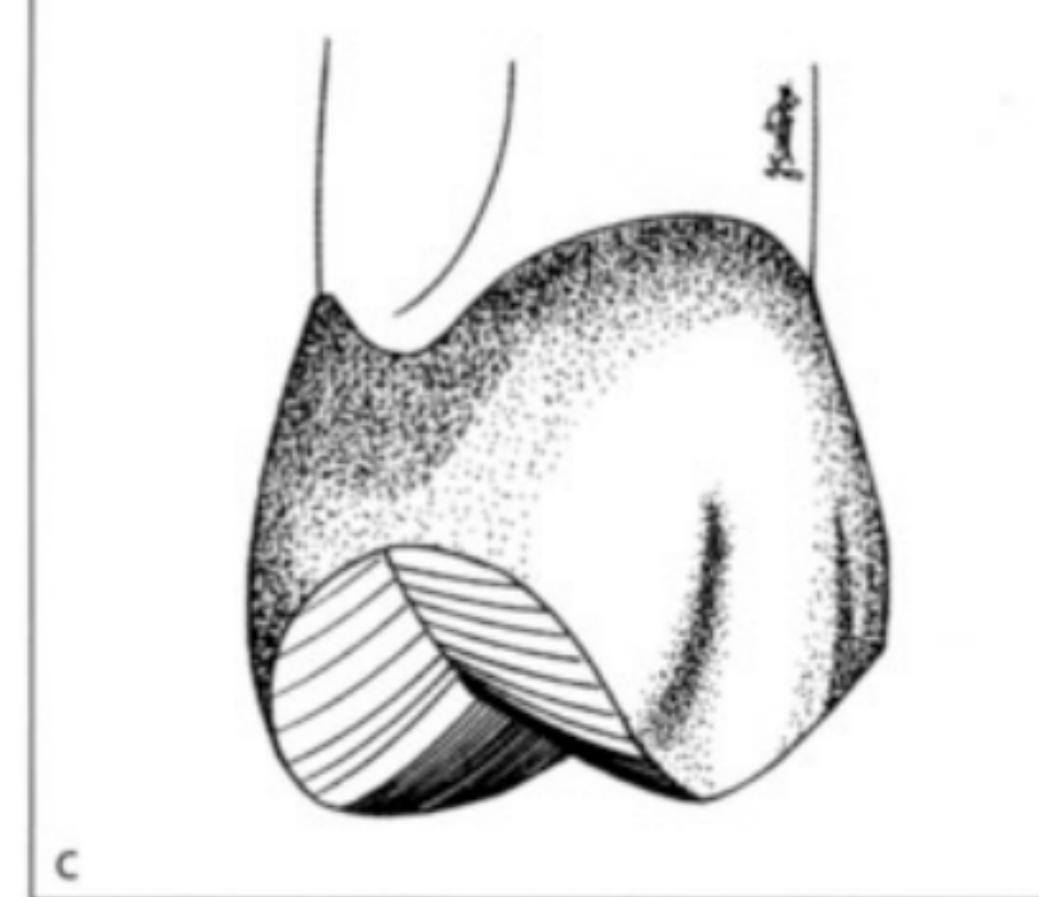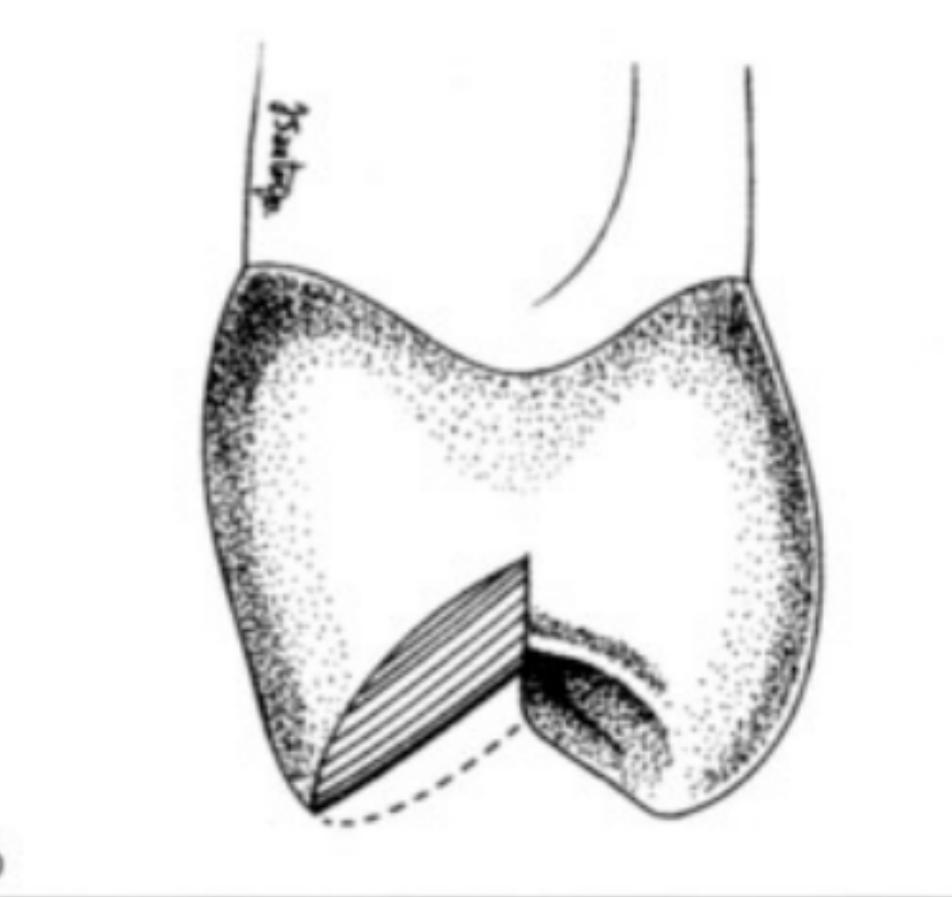

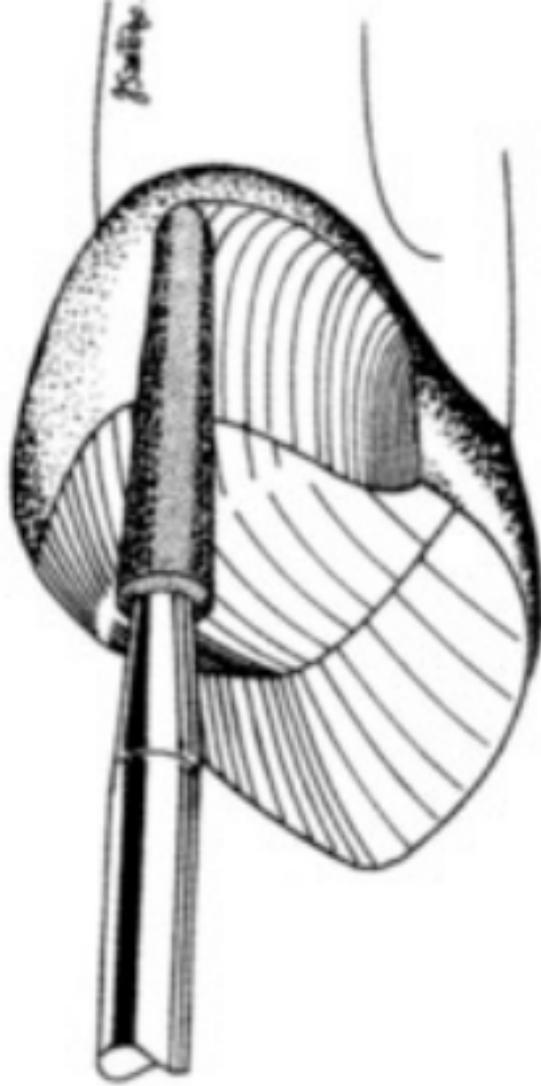

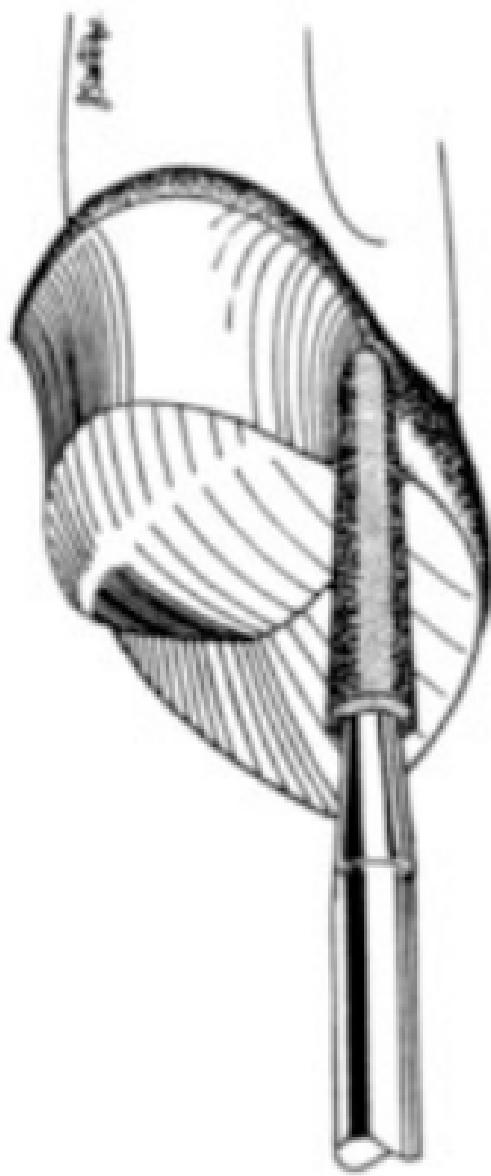

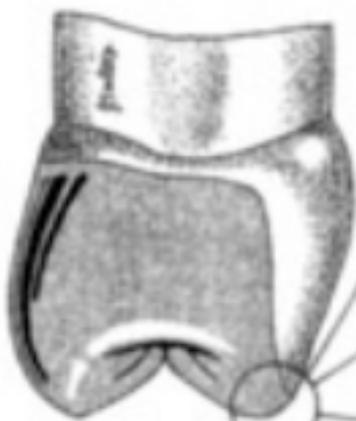


A


B

C




D

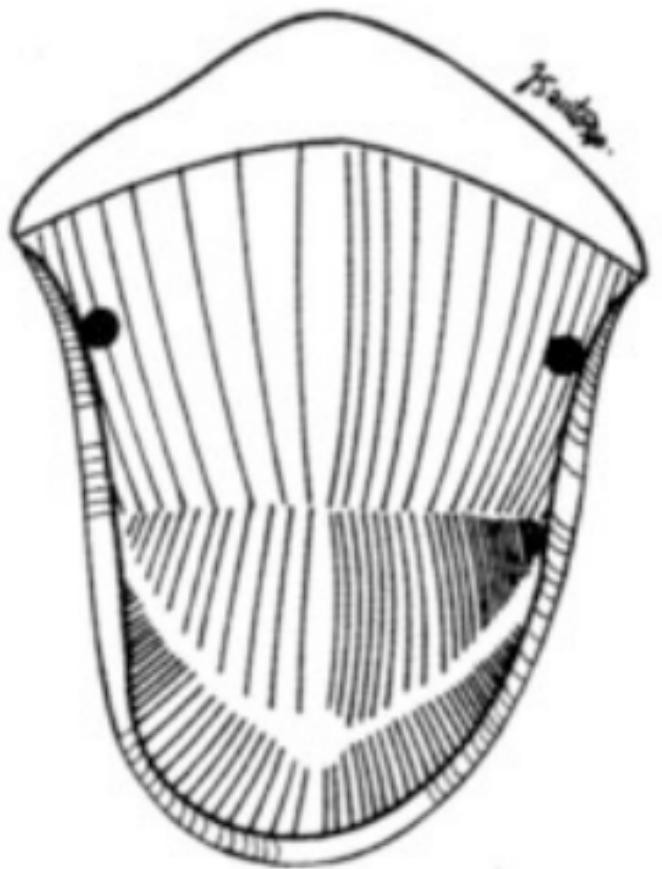



a



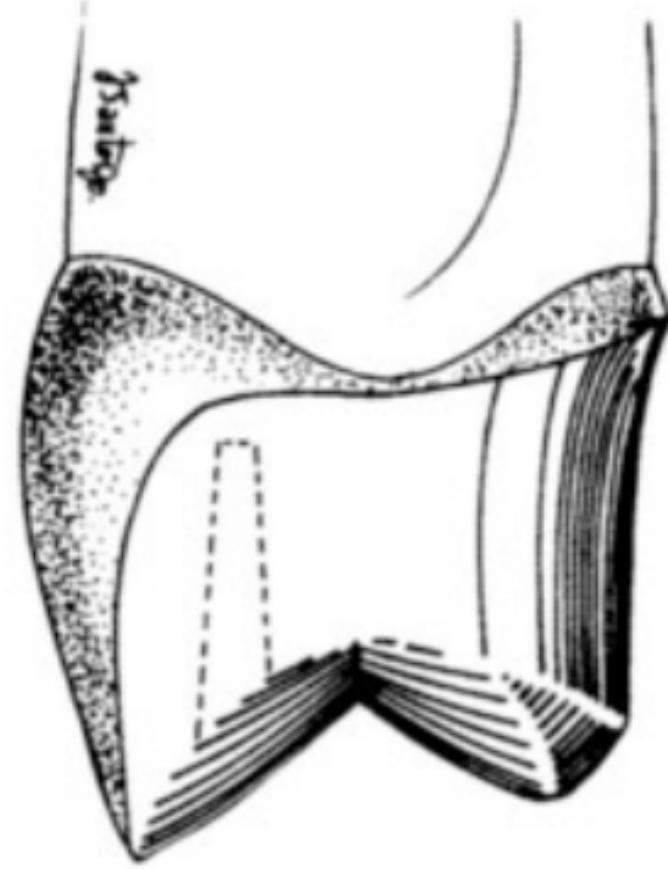



b

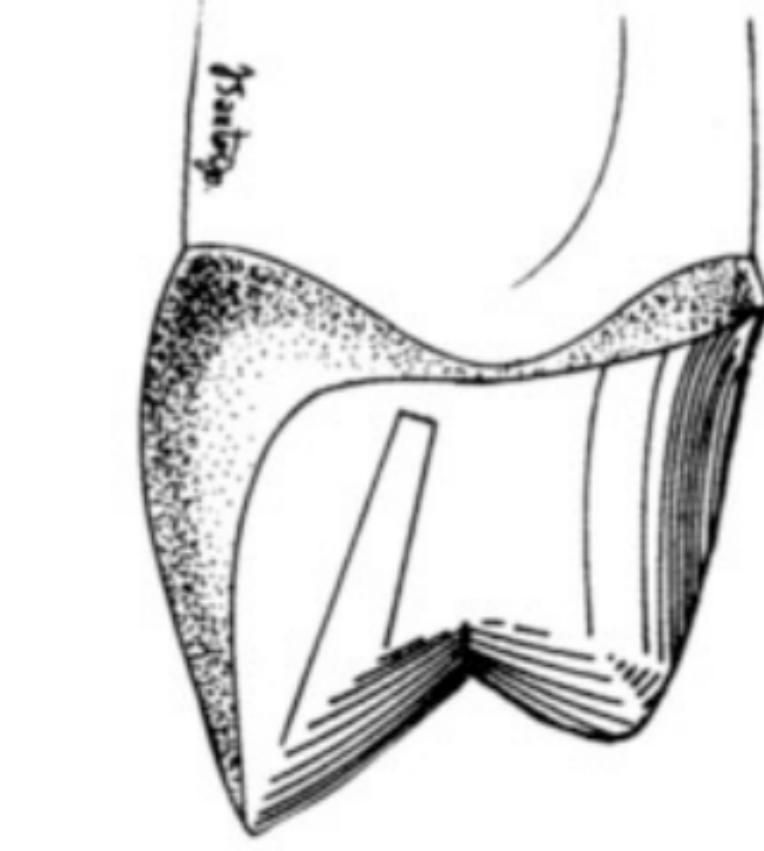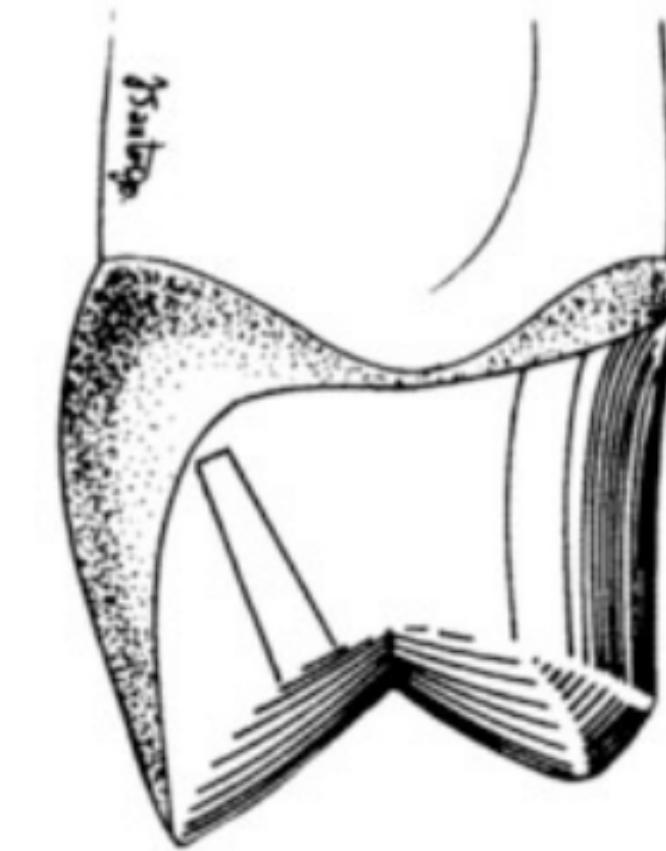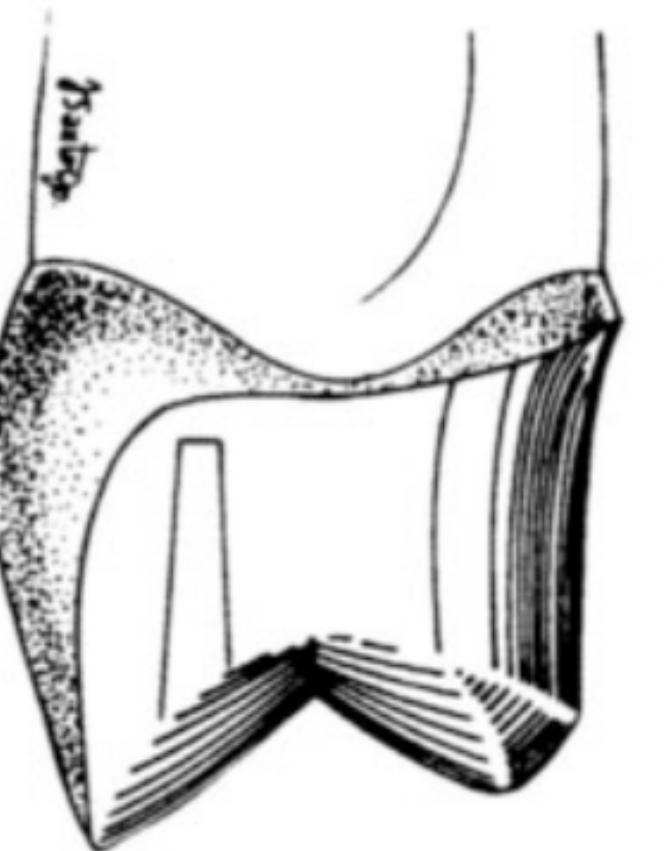

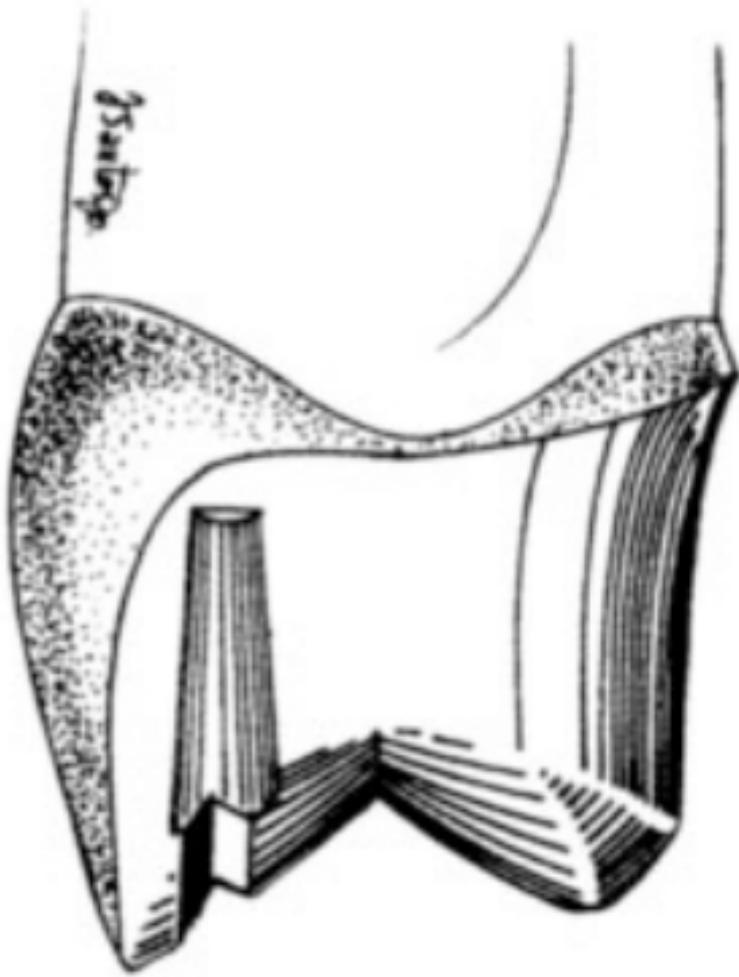


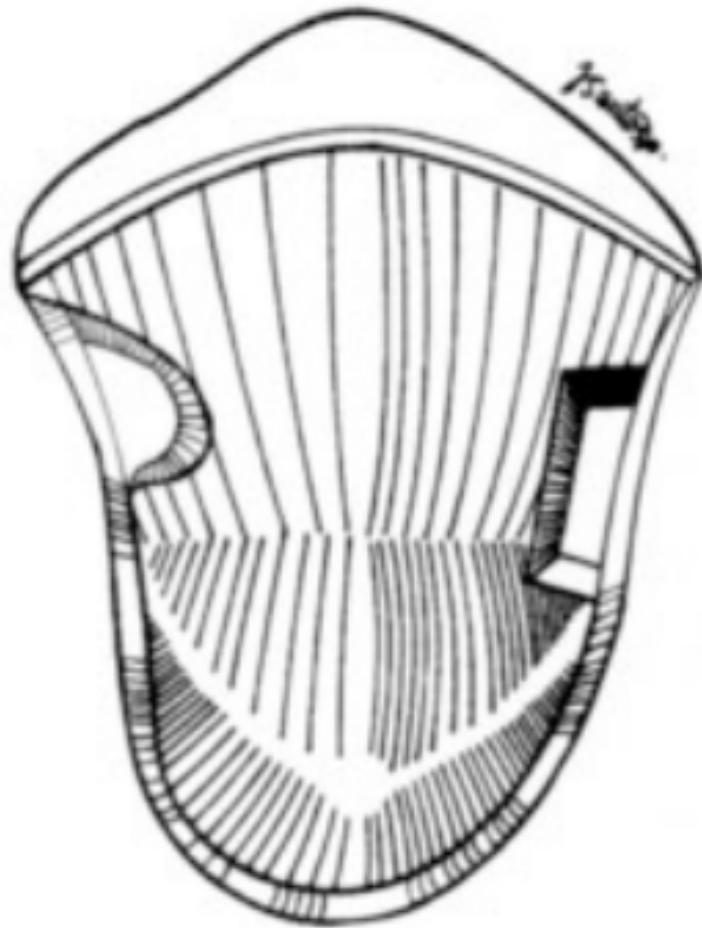

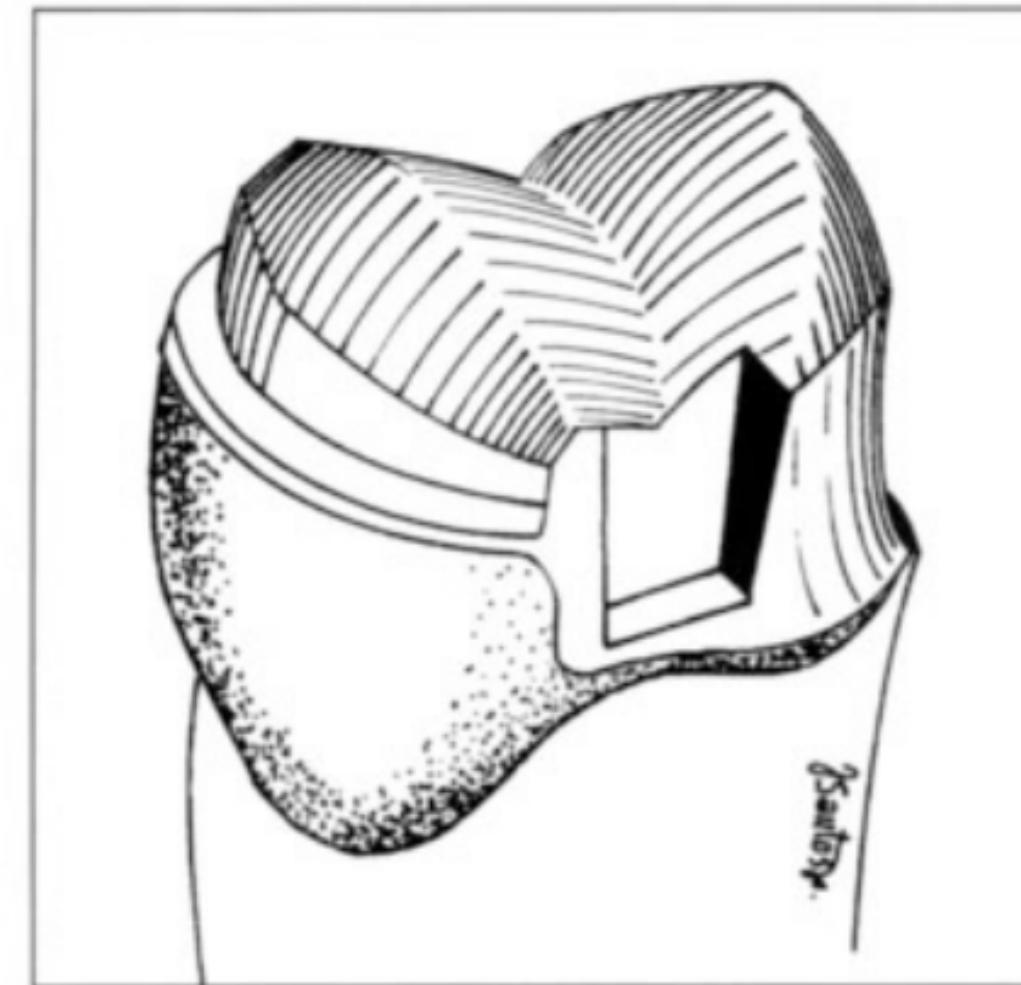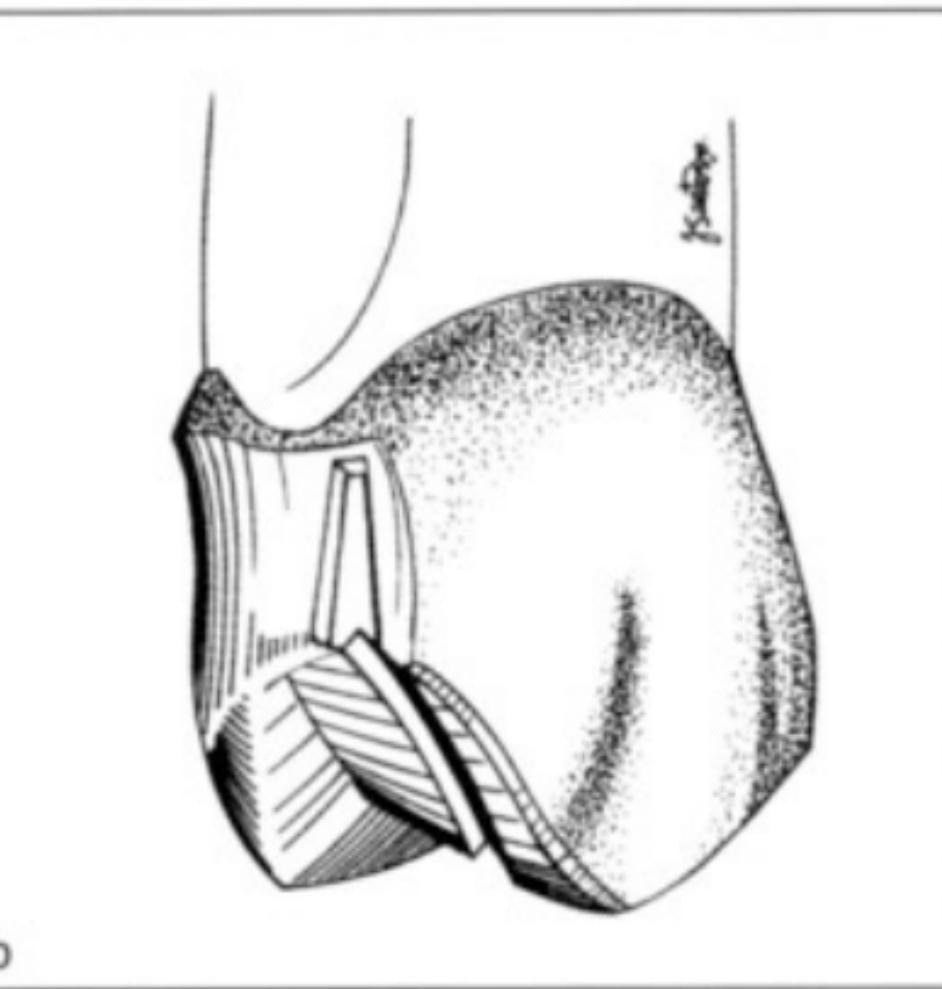
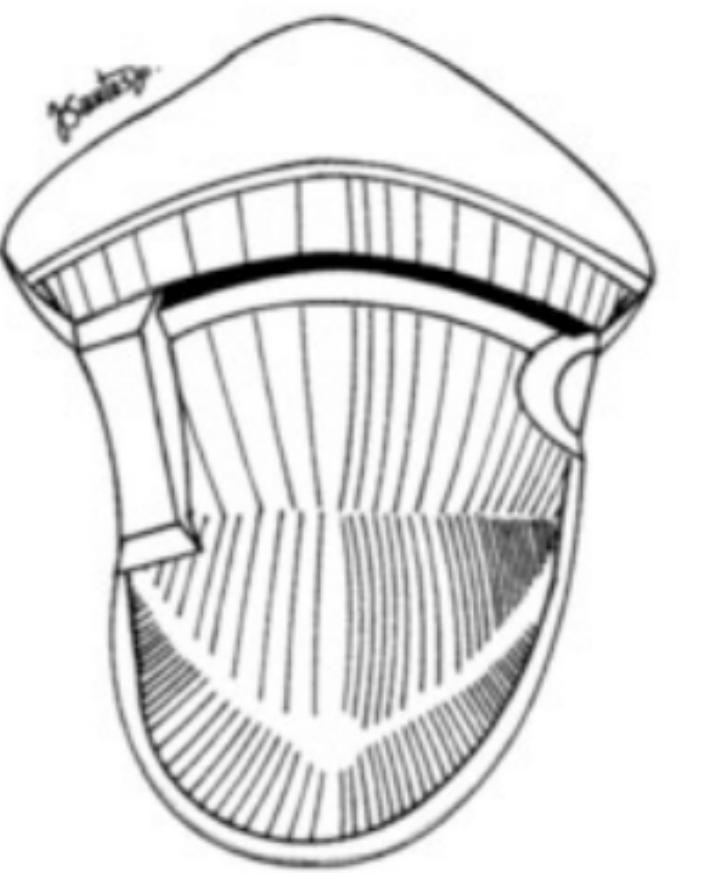


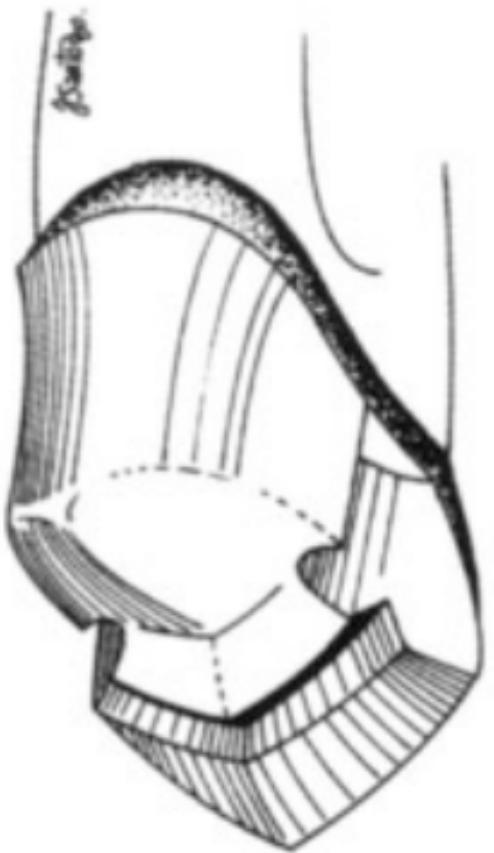


a

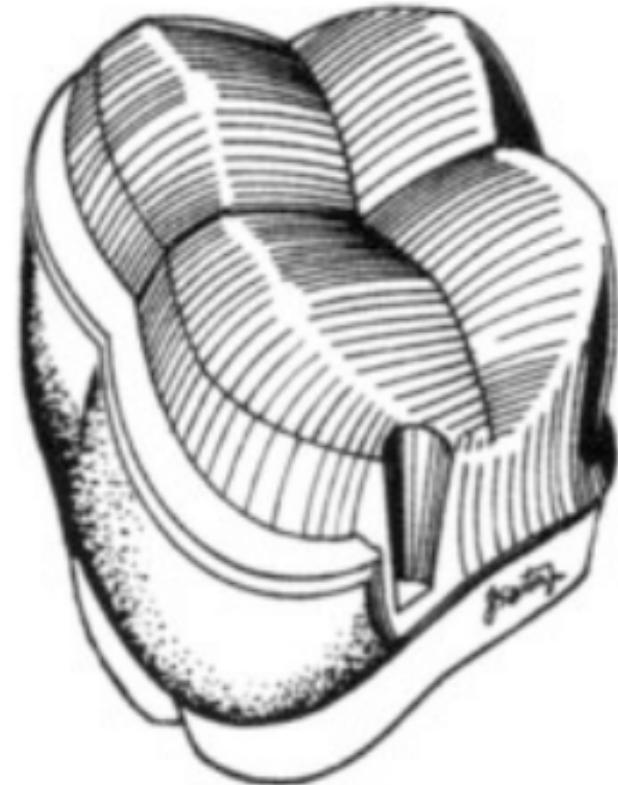

b

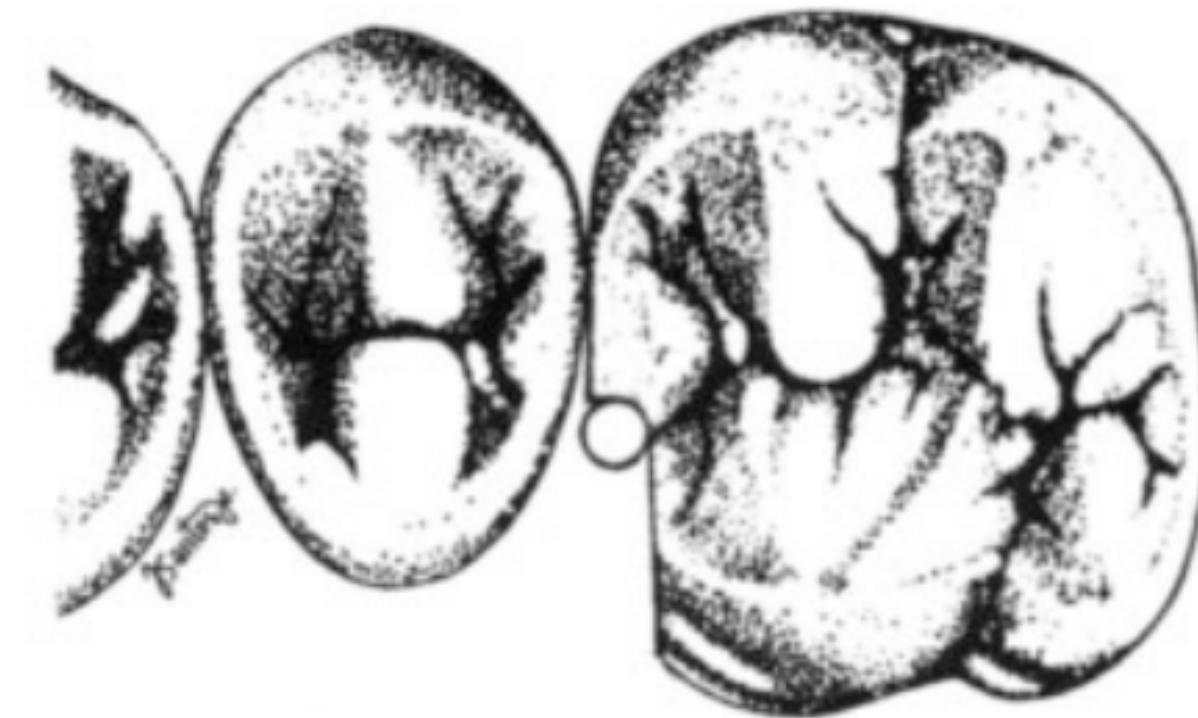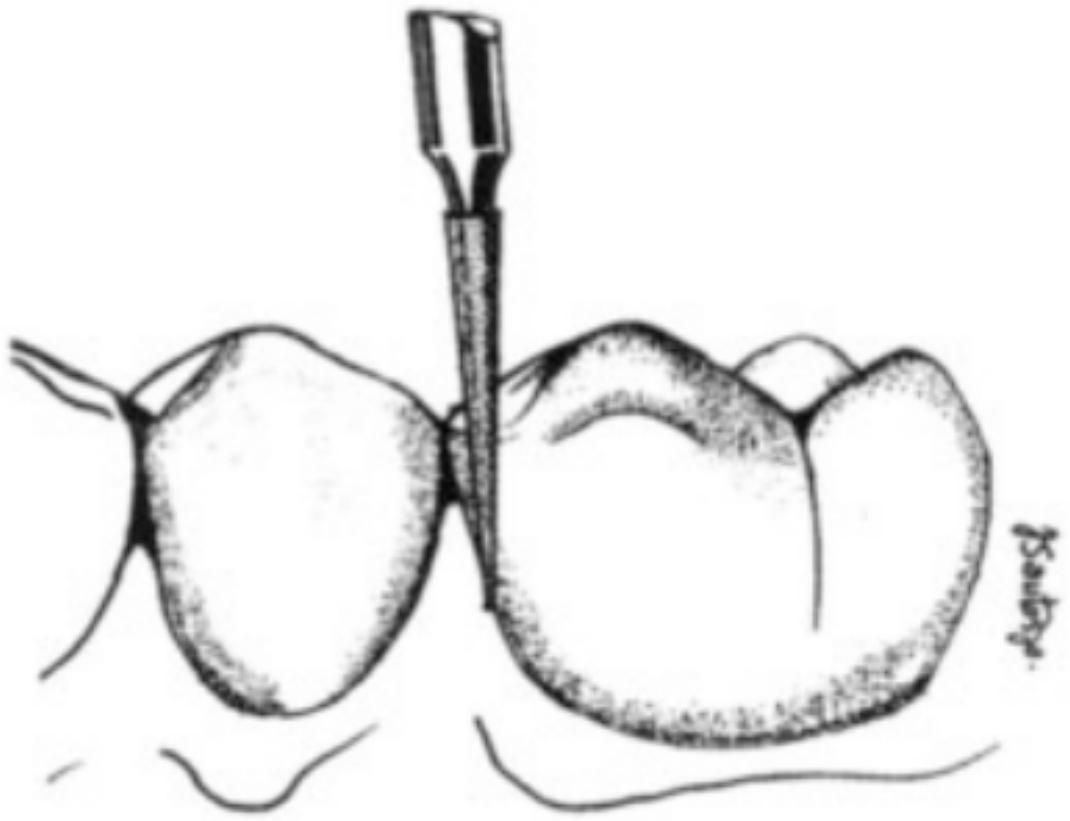

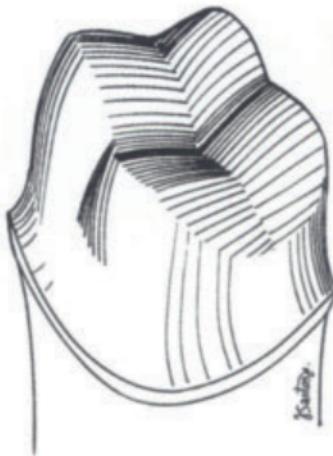

a




b



c



d

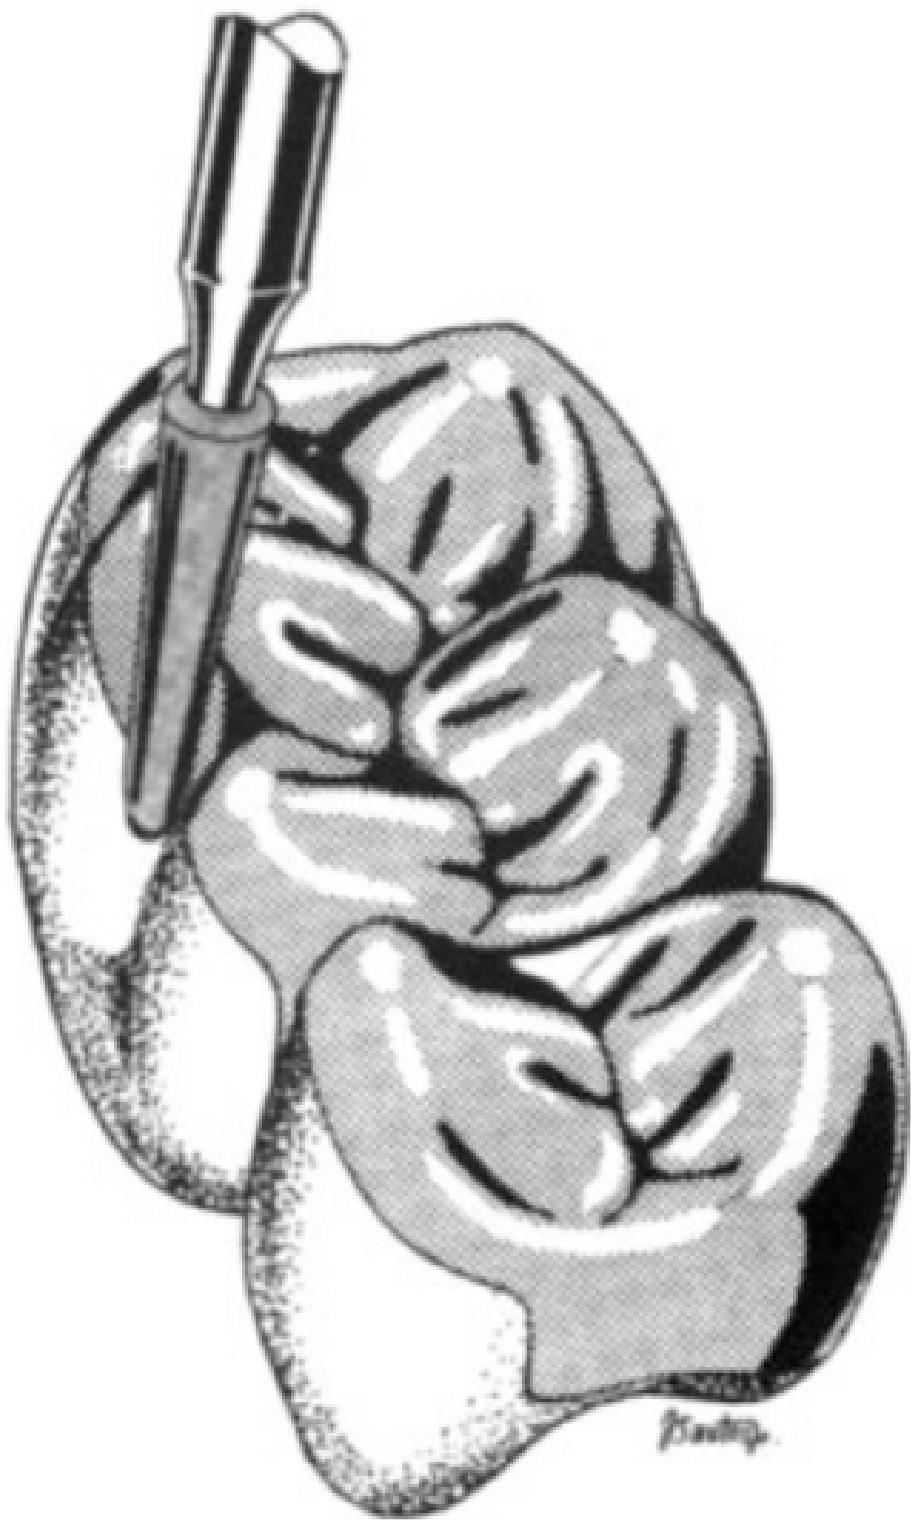



a



b



c

*Capture 21*



a



b










a




b

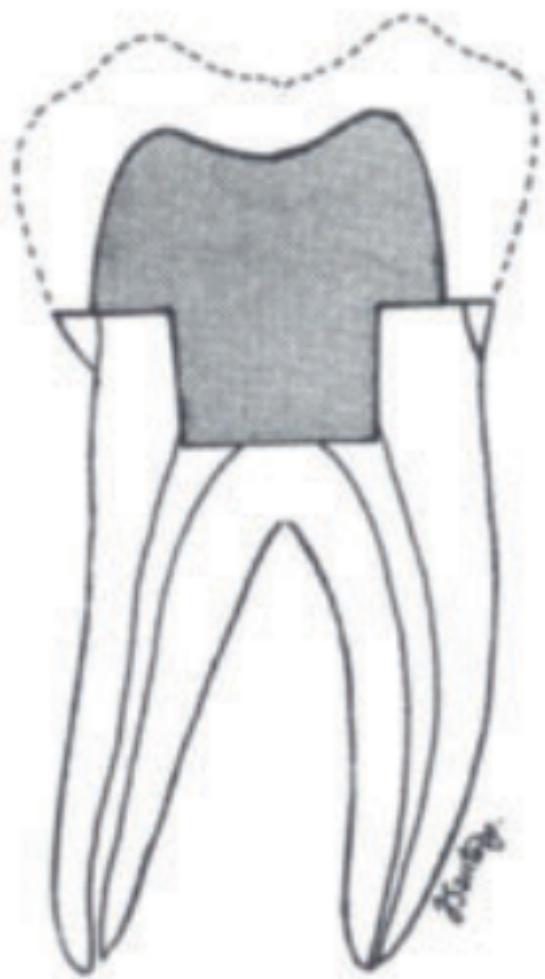

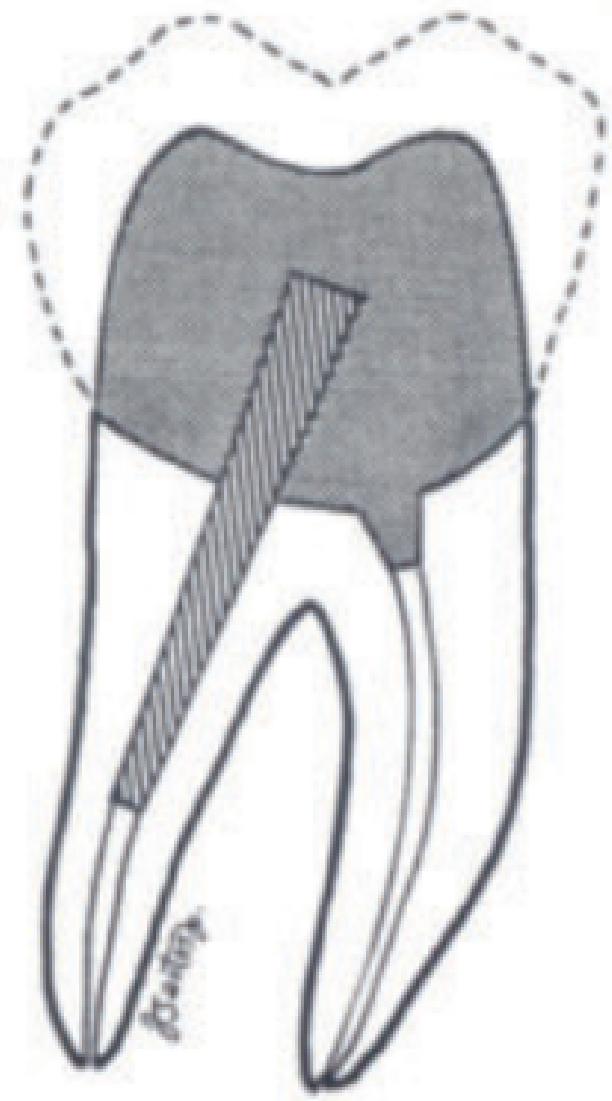


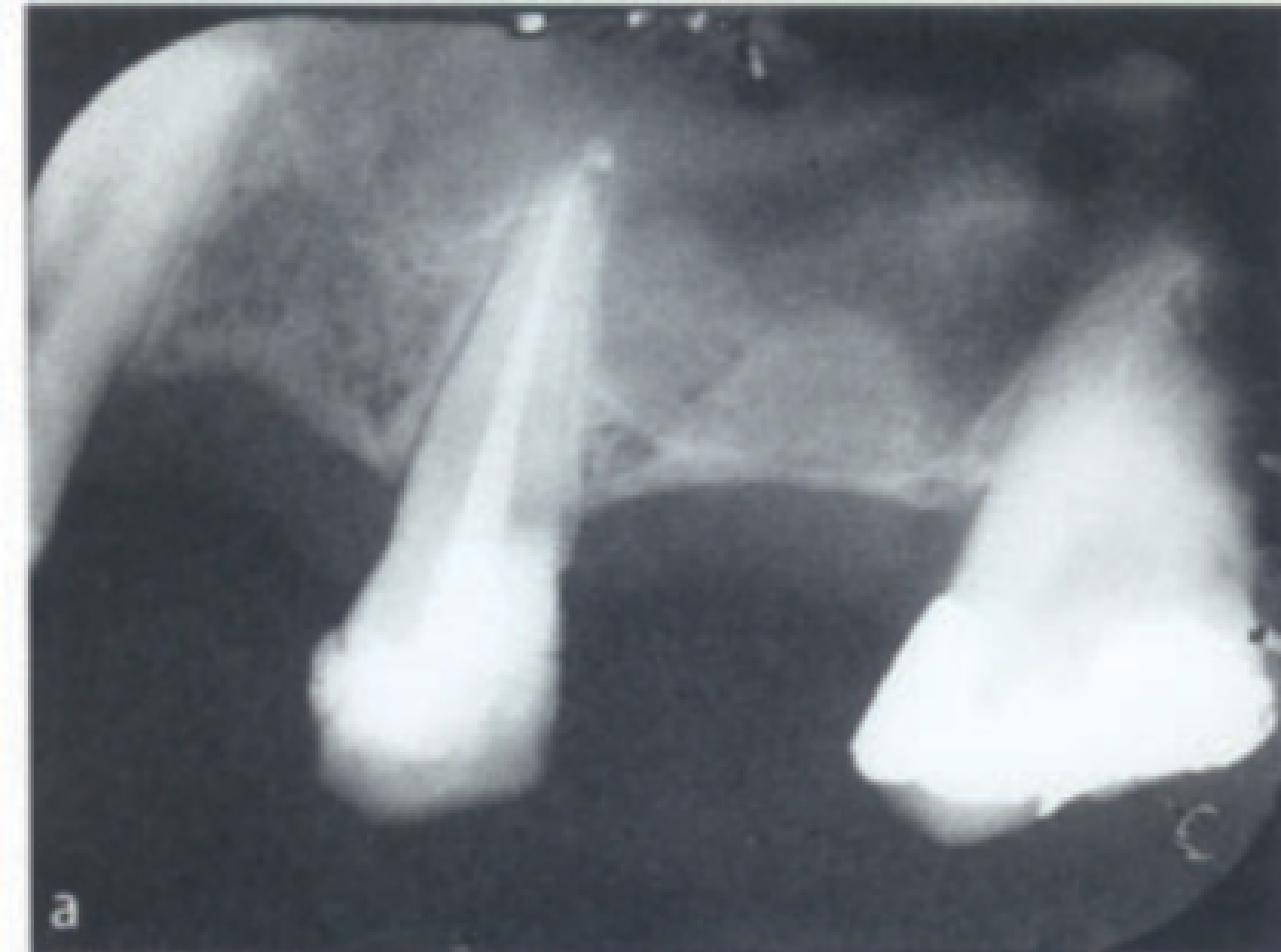




a

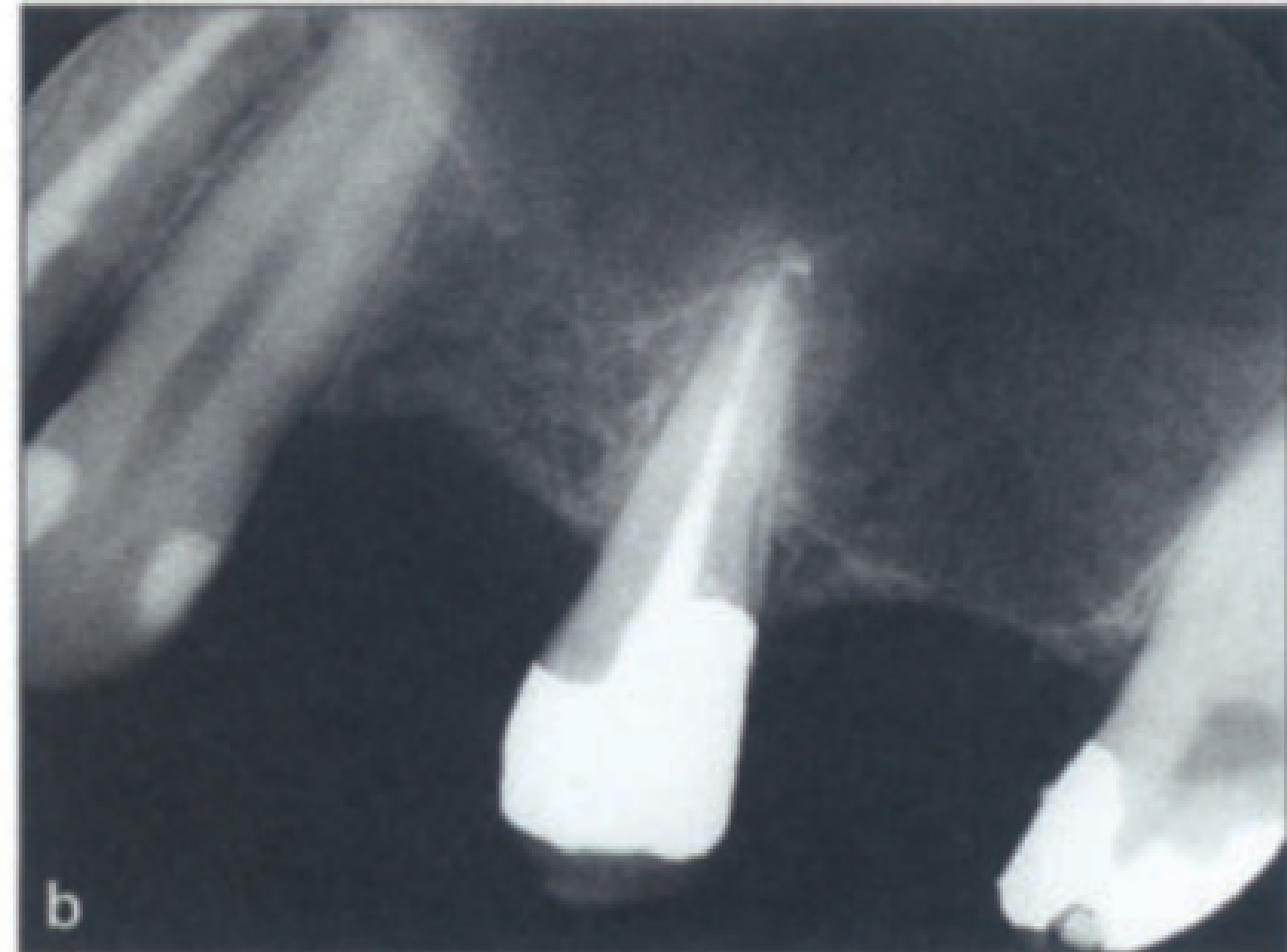

b



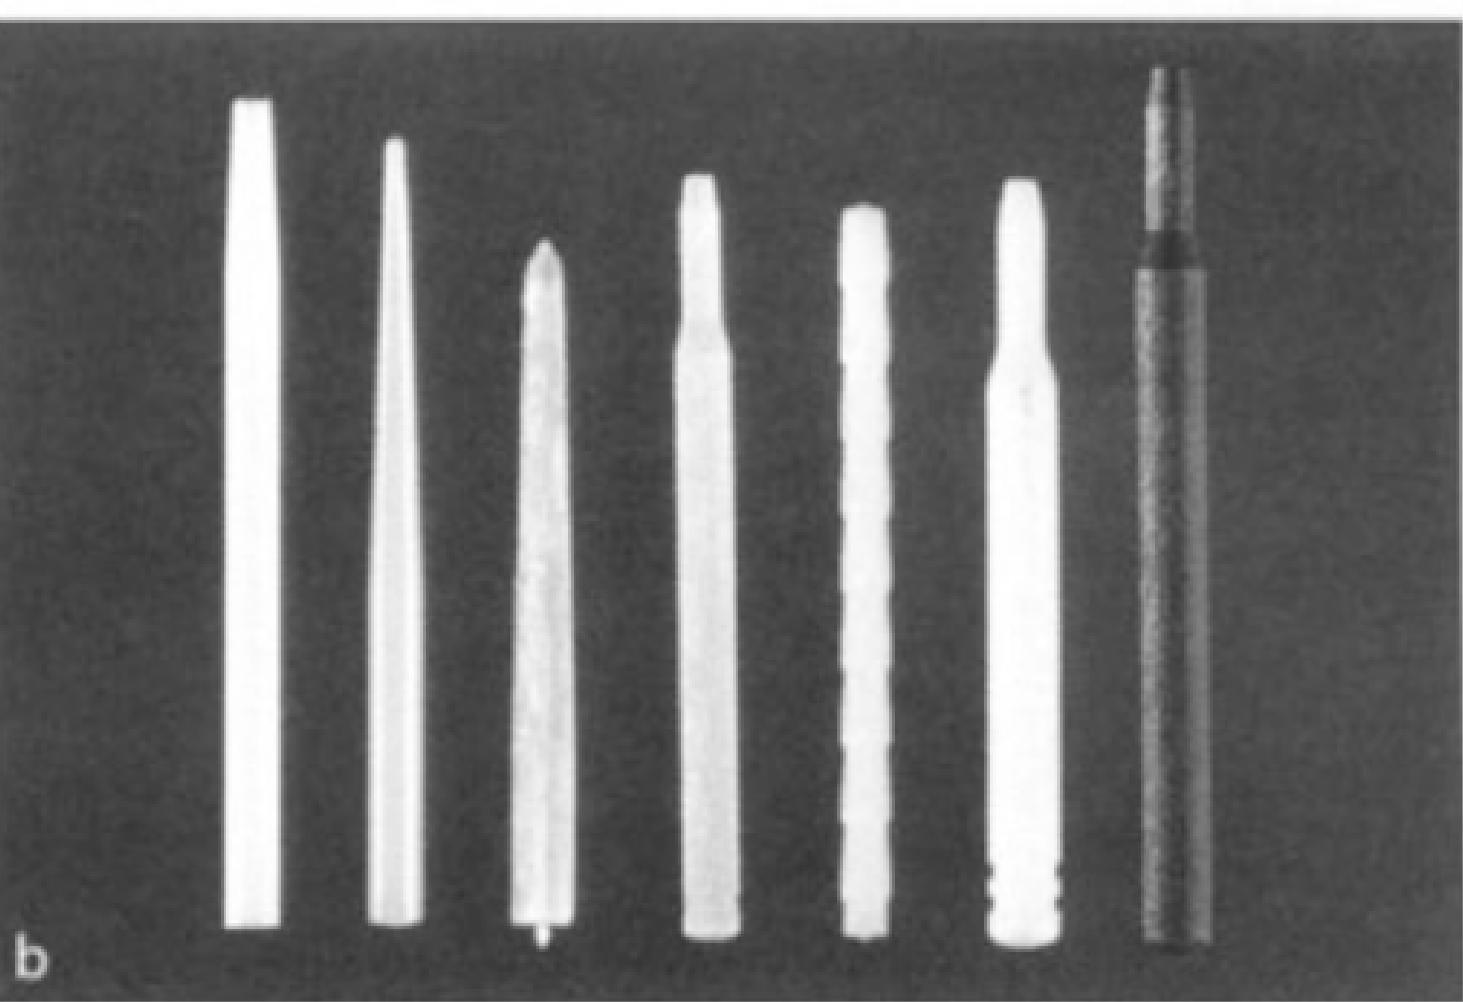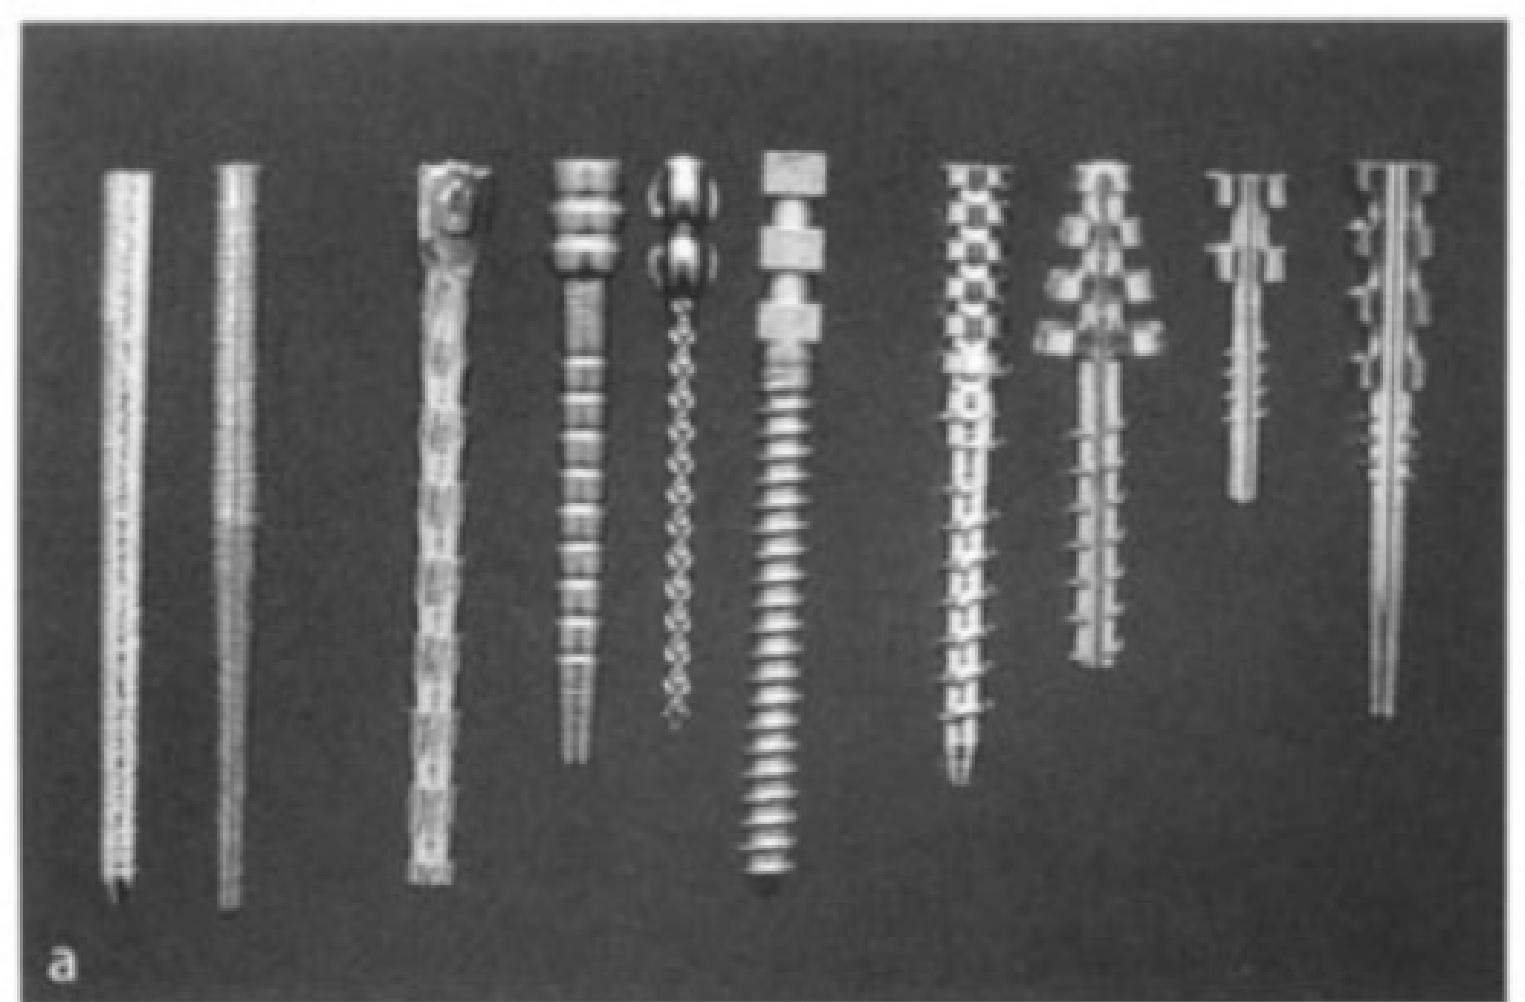

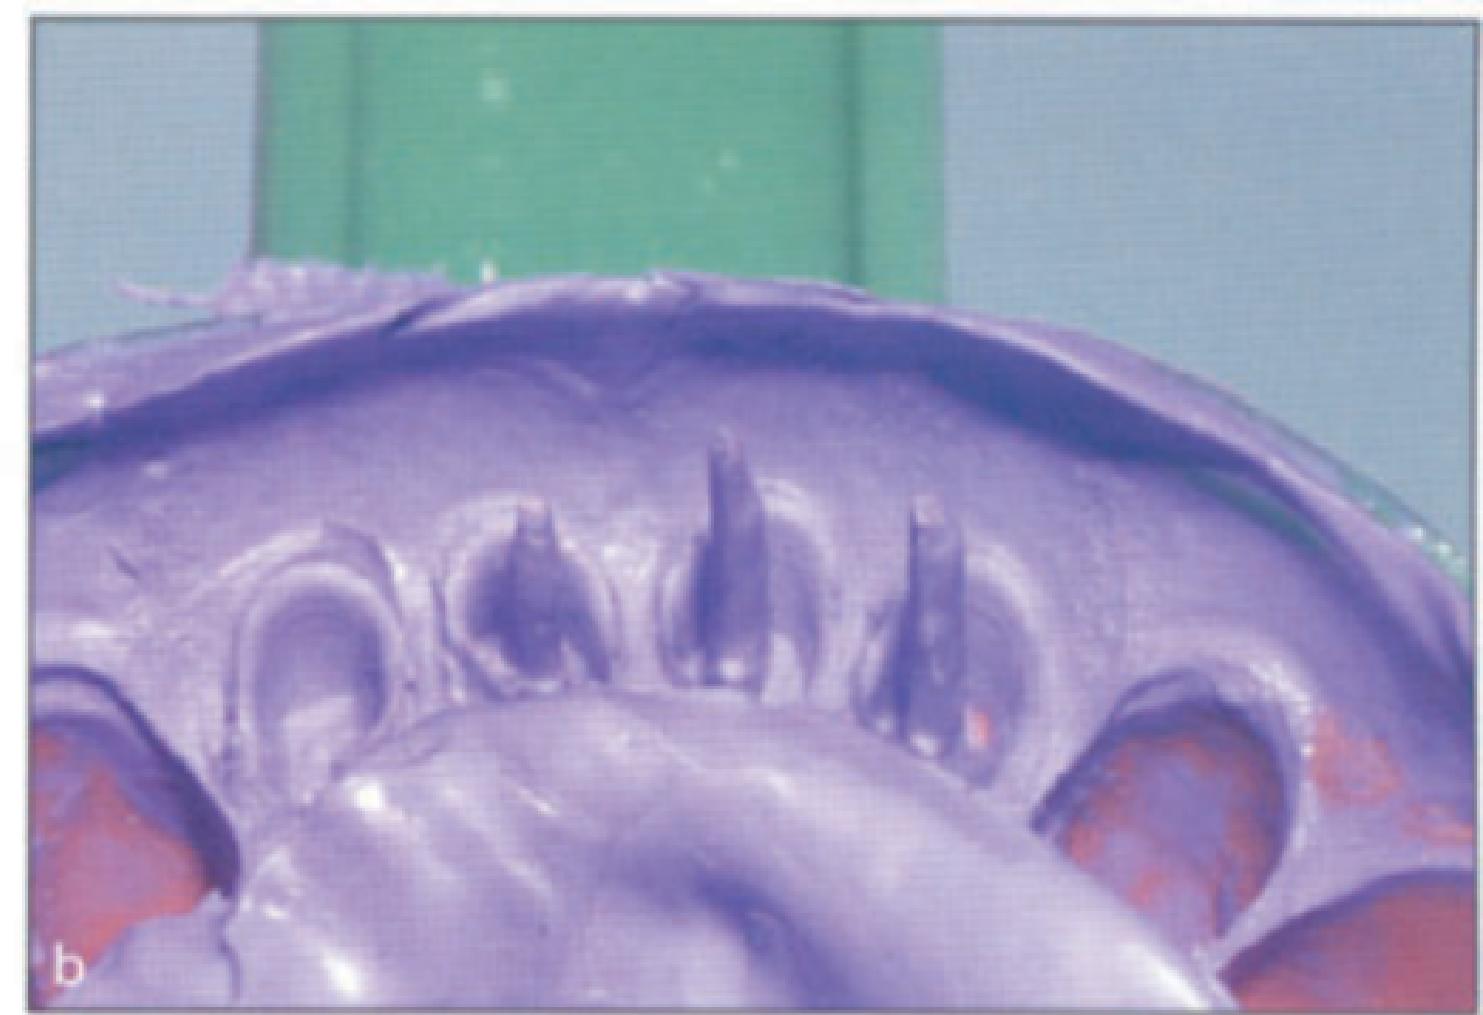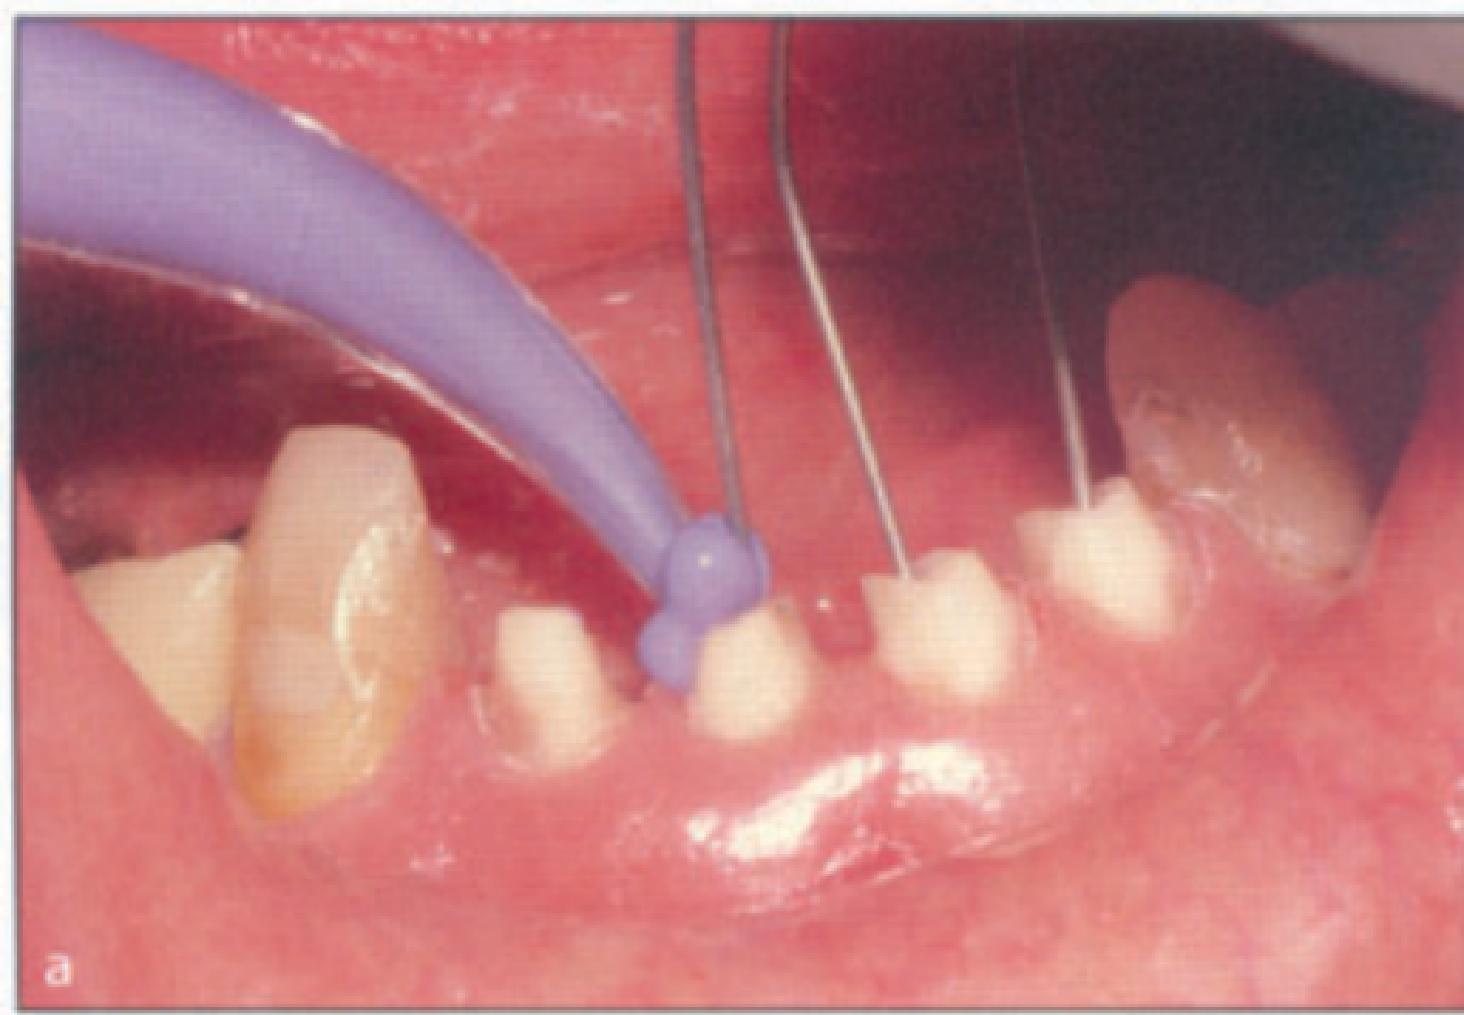



a




b




a

b



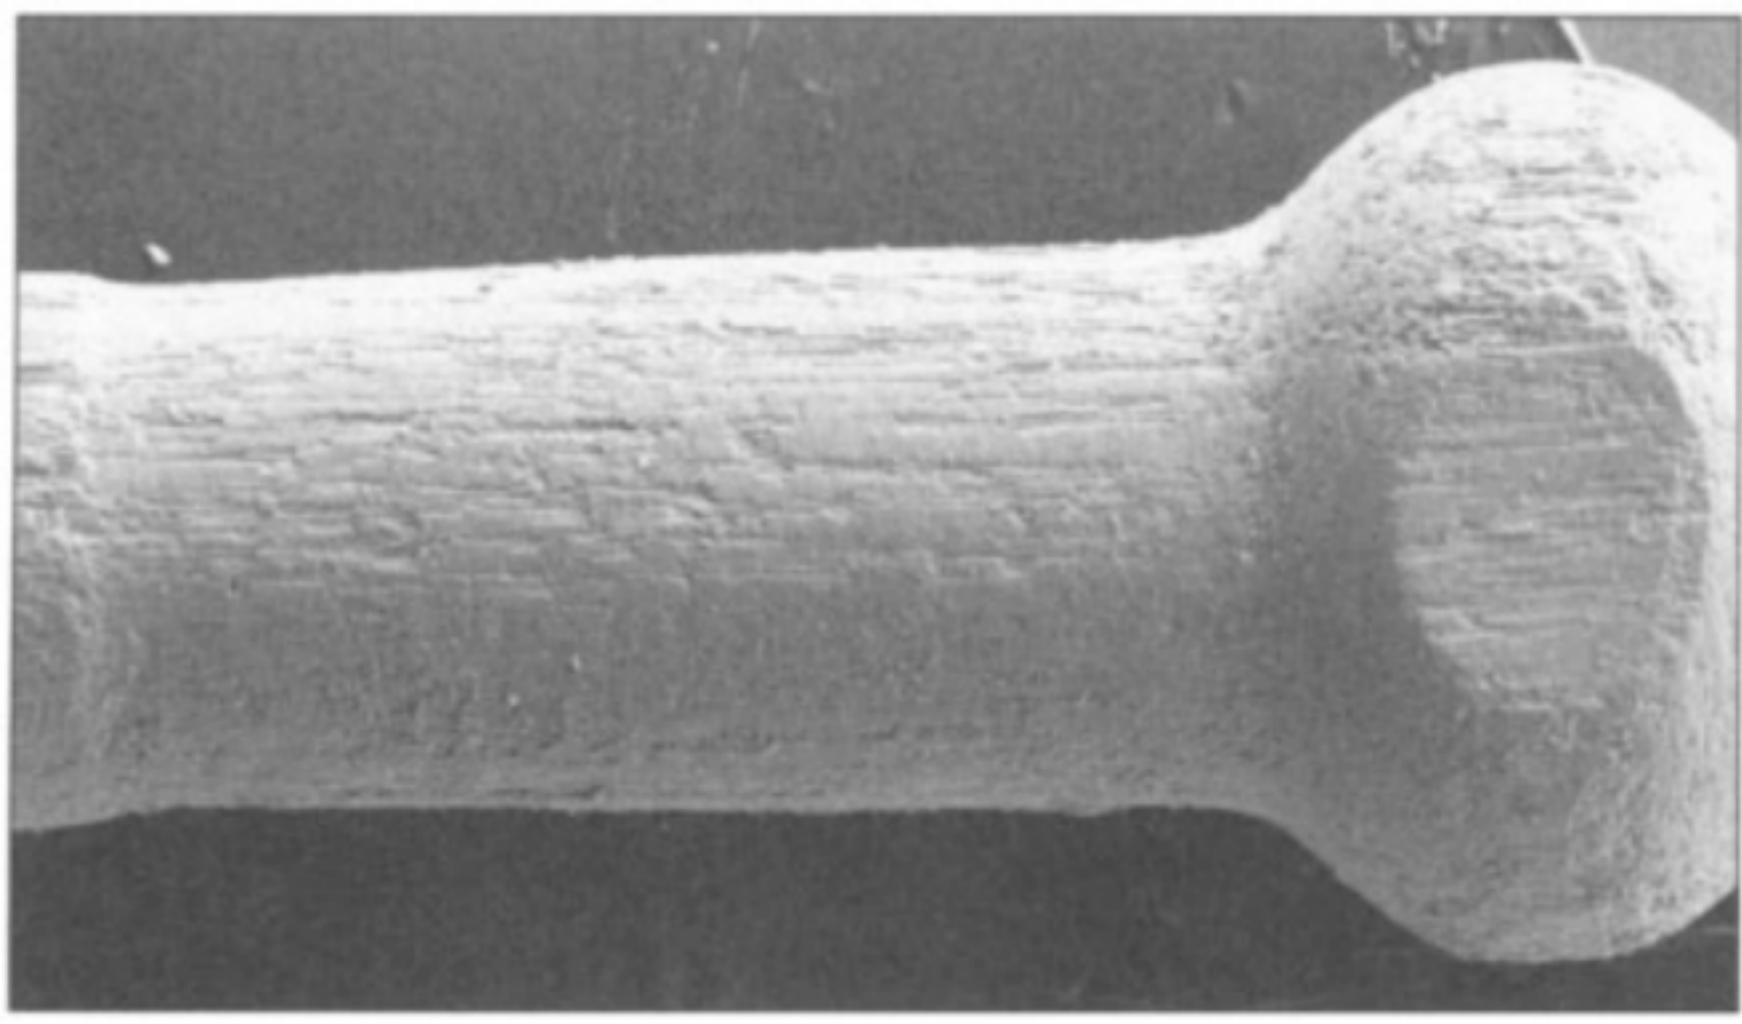


Functional force

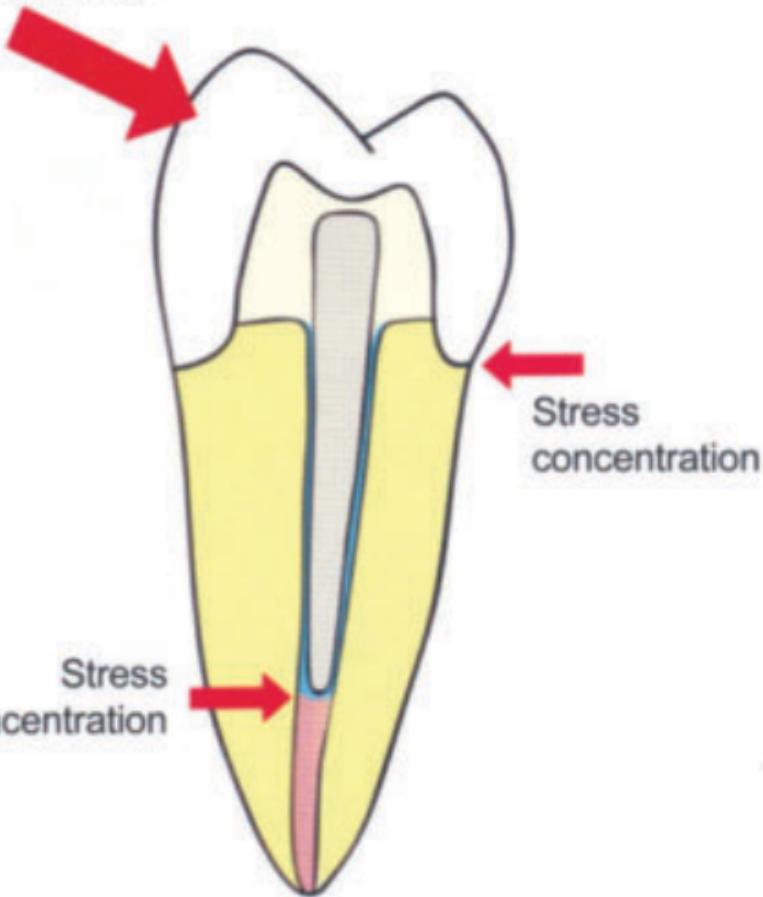





a


Functional force

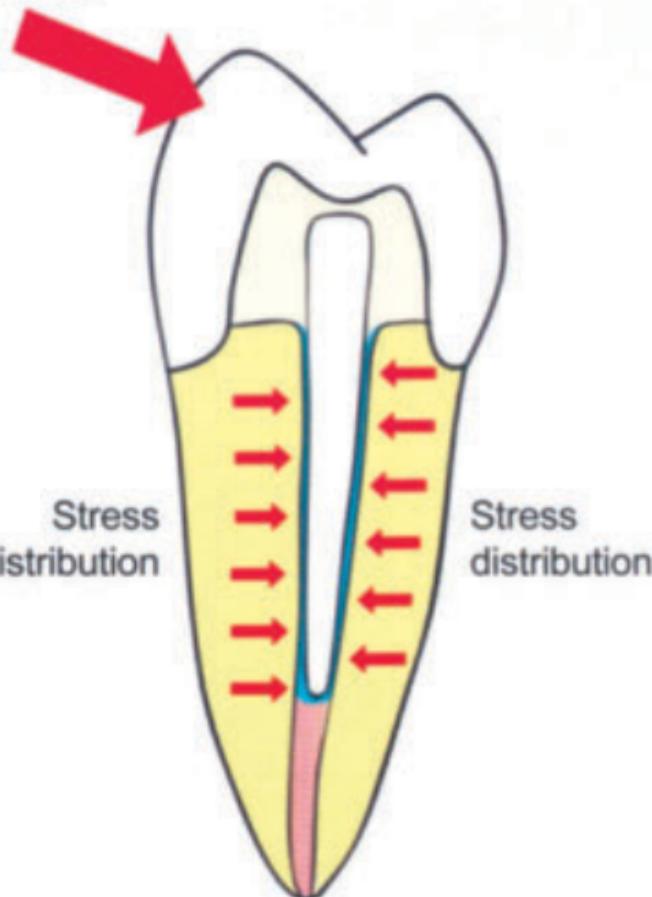

b

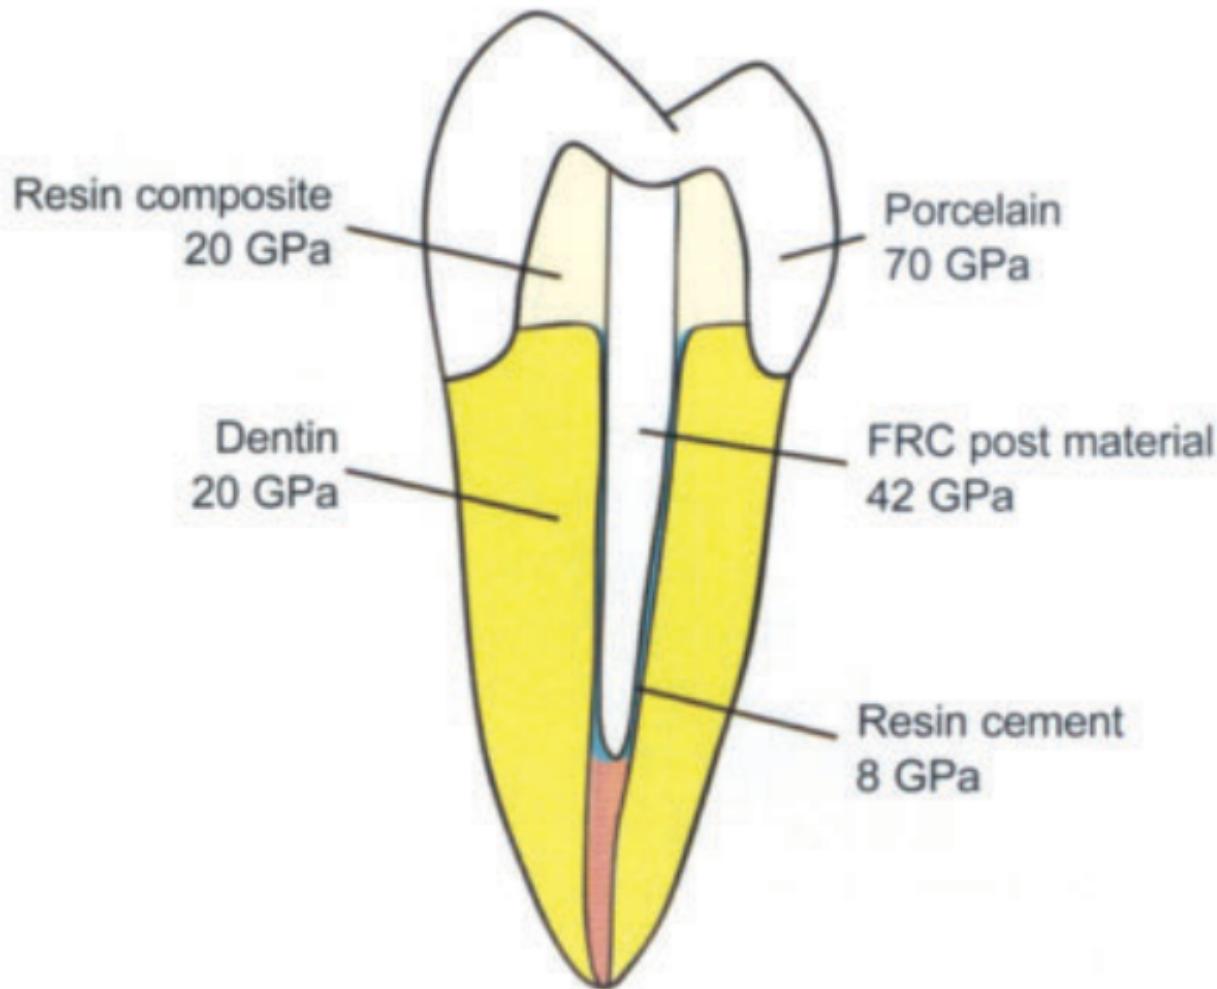

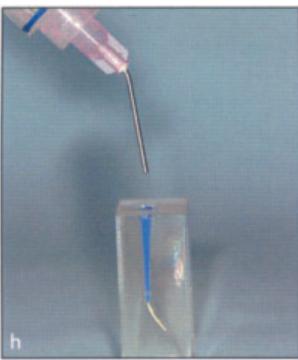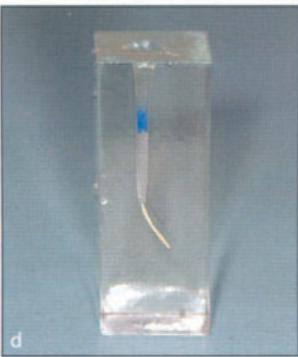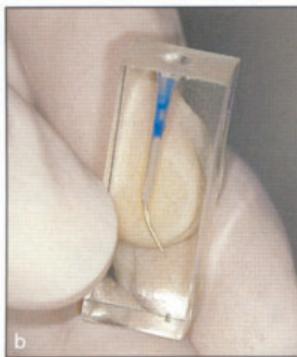


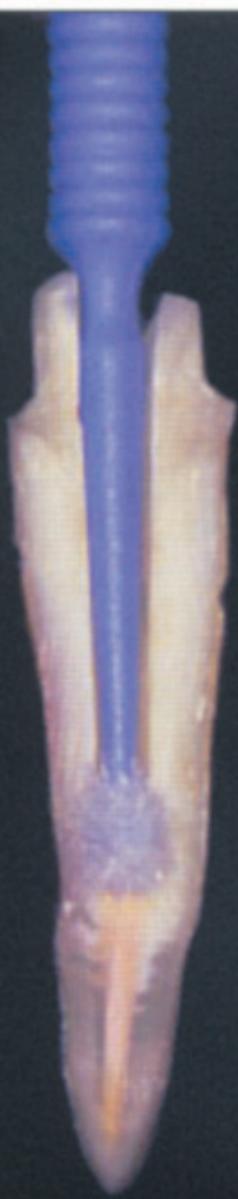

a



b

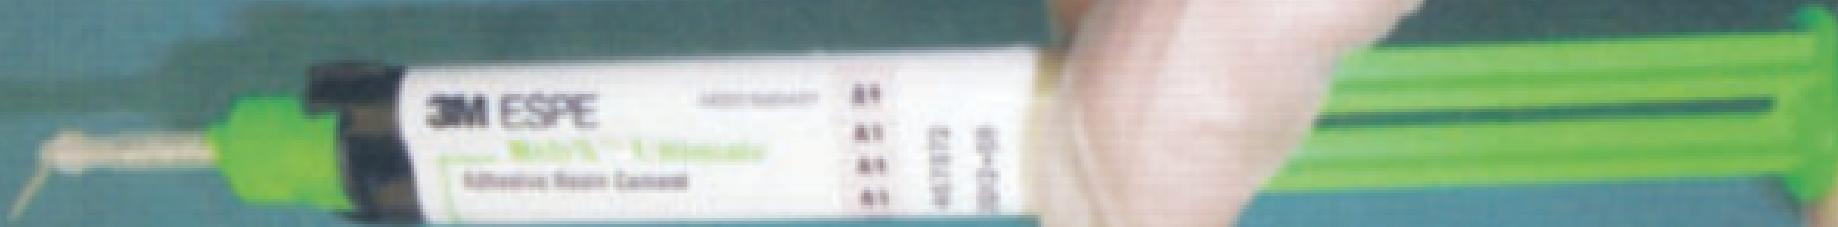

PerminFlo® DC

SYRINGE

10 ml



